

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020742.D
 Acq On : 24 Mar 2021 17:15
 Operator : SY/MD
 Sample : M1783-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	94	rVB	371344	365642	13.44%	1.743%
2	1.568	158	164	175	rVB	291635	320006	11.76%	1.526%
3	2.108	322	332	355	rVB	651093	974137	35.81%	4.645%
4	2.449	436	438	442	rVB3	1458	883	0.03%	0.004%
5	2.510	450	457	469	rBV7	5251	8726	0.32%	0.042%
6	2.687	508	512	514	rBV3	616	454	0.02%	0.002%
7	2.741	526	529	530	rBV2	594	332	0.01%	0.002%
8	2.764	534	536	537	rBV2	447	146	0.01%	0.001%
9	2.793	542	545	549	rVV3	491	329	0.01%	0.002%
10	2.957	594	596	597	rBV	462	158	0.01%	0.001%
11	3.011	611	613	615	rBV	600	279	0.01%	0.001%
12	3.069	630	631	634	rBV	287	150	0.01%	0.001%
13	3.082	634	635	636	rBV	499	173	0.01%	0.001%
14	3.108	641	643	647	rVV	498	283	0.01%	0.001%
15	3.285	696	698	701	rBV2	847	367	0.01%	0.002%
16	3.301	701	703	705	rBV3	342	157	0.01%	0.001%
17	3.394	729	732	735	rVB3	770	437	0.02%	0.002%
18	3.452	748	750	751	rBV	398	147	0.01%	0.001%
19	3.462	751	753	756	rVB3	616	366	0.01%	0.002%
20	3.474	756	757	759	rBV2	499	244	0.01%	0.001%
21	3.507	764	767	768	rBV2	178	90	0.00%	0.000%
22	3.519	768	771	773	rBV	702	613	0.02%	0.003%
23	3.584	790	791	794	rBV	408	230	0.01%	0.001%
24	3.626	801	804	809	rBV3	864	585	0.02%	0.003%
25	3.654	809	813	815	rBV3	586	524	0.02%	0.002%
26	3.709	828	830	831	rVB	337	105	0.00%	0.001%
27	3.719	831	833	835	rBV2	459	296	0.01%	0.001%
28	3.748	841	842	844	rBV	308	144	0.01%	0.001%
29	3.777	848	851	852	rBV	310	174	0.01%	0.001%
30	3.812	858	862	864	rBV	488	360	0.01%	0.002%
31	3.825	864	866	870	rVB5	913	519	0.02%	0.002%
32	3.889	875	886	920	rBV	180118	517450	19.02%	2.467%
33	4.352	1014	1030	1062	rBV	459202	1137206	41.80%	5.422%
34	4.831	1173	1179	1180	rBV4	718	598	0.02%	0.003%
35	4.896	1197	1199	1203	rVB3	1311	834	0.03%	0.004%
36	4.947	1213	1215	1217	rBV3	650	321	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032421\
 Data File : VW020742.D
 Acq On : 24 Mar 2021 17:15
 Operator : SY/MD
 Sample : M1783-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.050	1230	1247	1273	rBV2	1060889	2720506	100.00%	12.972%
38	5.622	1411	1425	1454	rBV	852823	1725210	63.42%	8.226%
39	5.998	1540	1542	1543	rBV	480	169	0.01%	0.001%
40	6.076	1551	1566	1586	rBV	582284	1196918	44.00%	5.707%
41	6.346	1648	1650	1652	rBV	1240	753	0.03%	0.004%
42	6.384	1659	1662	1664	rBV2	907	569	0.02%	0.003%
43	6.513	1700	1702	1706	rBV2	462	327	0.01%	0.002%
44	6.561	1714	1717	1718	rBV3	855	382	0.01%	0.002%
45	6.622	1733	1736	1738	rBV3	903	578	0.02%	0.003%
46	6.670	1747	1751	1754	rBV3	1302	1193	0.04%	0.006%
47	6.693	1754	1758	1760	rVV5	986	800	0.03%	0.004%
48	6.764	1778	1780	1782	rBV2	868	492	0.02%	0.002%
49	6.783	1783	1786	1789	rVB2	949	579	0.02%	0.003%
50	6.815	1792	1796	1798	rBV3	716	532	0.02%	0.003%
51	6.847	1803	1806	1812	rVV5	916	808	0.03%	0.004%
52	6.879	1813	1816	1818	rVV3	703	438	0.02%	0.002%
53	6.892	1818	1820	1824	rVV3	996	601	0.02%	0.003%
54	6.912	1824	1826	1829	rVB2	682	346	0.01%	0.002%
55	6.989	1839	1850	1875	rBV	334341	609633	22.41%	2.907%
56	7.188	1909	1912	1914	rBV2	1093	747	0.03%	0.004%
57	7.320	1941	1953	1981	rBV	1245307	2148669	78.98%	10.245%
58	7.625	2035	2048	2071	rBV	239657	424374	15.60%	2.023%
59	8.092	2182	2193	2221	rBV	677111	1194229	43.90%	5.694%
60	8.748	2396	2397	2398	rBB	370	143	0.01%	0.001%
61	8.789	2403	2410	2413	rBV7	1223	1503	0.06%	0.007%
62	8.857	2419	2431	2464	rBV	1302338	2118165	77.86%	10.100%
63	9.262	2555	2557	2558	rVB	365	80	0.00%	0.000%
64	9.391	2595	2597	2599	rBV3	843	383	0.01%	0.002%
65	9.680	2685	2687	2688	rBV2	803	251	0.01%	0.001%
66	9.728	2700	2702	2703	rBV	549	229	0.01%	0.001%
67	9.838	2734	2736	2741	rVB3	647	452	0.02%	0.002%
68	9.863	2741	2744	2747	rBV3	1115	838	0.03%	0.004%
69	10.043	2798	2800	2802	rBV2	999	519	0.02%	0.002%
70	10.098	2816	2817	2821	rBV3	508	322	0.01%	0.002%
71	10.120	2821	2824	2825	rBV2	498	251	0.01%	0.001%
72	10.165	2835	2838	2840	rBV2	894	455	0.02%	0.002%
73	10.178	2840	2842	2843	rBV	485	185	0.01%	0.001%
74	10.220	2843	2855	2876	rBV	842016	1319786	48.51%	6.293%
75	10.378	2901	2904	2908	rBV4	769	786	0.03%	0.004%
76	10.548	2952	2957	2959	rBV3	1151	931	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020742.D
 Acq On : 24 Mar 2021 17:15
 Operator : SY/MD
 Sample : M1783-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.654	2988	2990	2991	rBV	556	192	0.01%	0.001%
78	10.905	3065	3068	3070	rBV2	946	563	0.02%	0.003%
79	11.046	3109	3112	3114	rBV2	1094	675	0.02%	0.003%
80	11.075	3118	3121	3124	rVB3	822	520	0.02%	0.002%
81	11.130	3135	3138	3143	rBV3	1084	968	0.04%	0.005%
82	11.255	3165	3177	3199	rBV	1355134	2083366	76.58%	9.934%
83	11.628	3281	3293	3311	rBV	1308198	2073265	76.21%	9.886%
84	12.059	3425	3427	3431	rBV3	710	484	0.02%	0.002%
85	12.243	3479	3484	3488	rBV4	935	1040	0.04%	0.005%
86	12.403	3531	3534	3536	rBV2	1005	619	0.02%	0.003%
87	12.519	3566	3570	3573	rBV4	1189	1196	0.04%	0.006%
88	12.664	3611	3615	3620	rBV4	1341	1149	0.04%	0.005%
89	12.763	3644	3646	3650	rBV4	1127	720	0.03%	0.003%


Sum of corrected areas: 20972354

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020742.D
Acq On : 24 Mar 2021 17:15
Operator : SY/MD
Sample : M1783-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

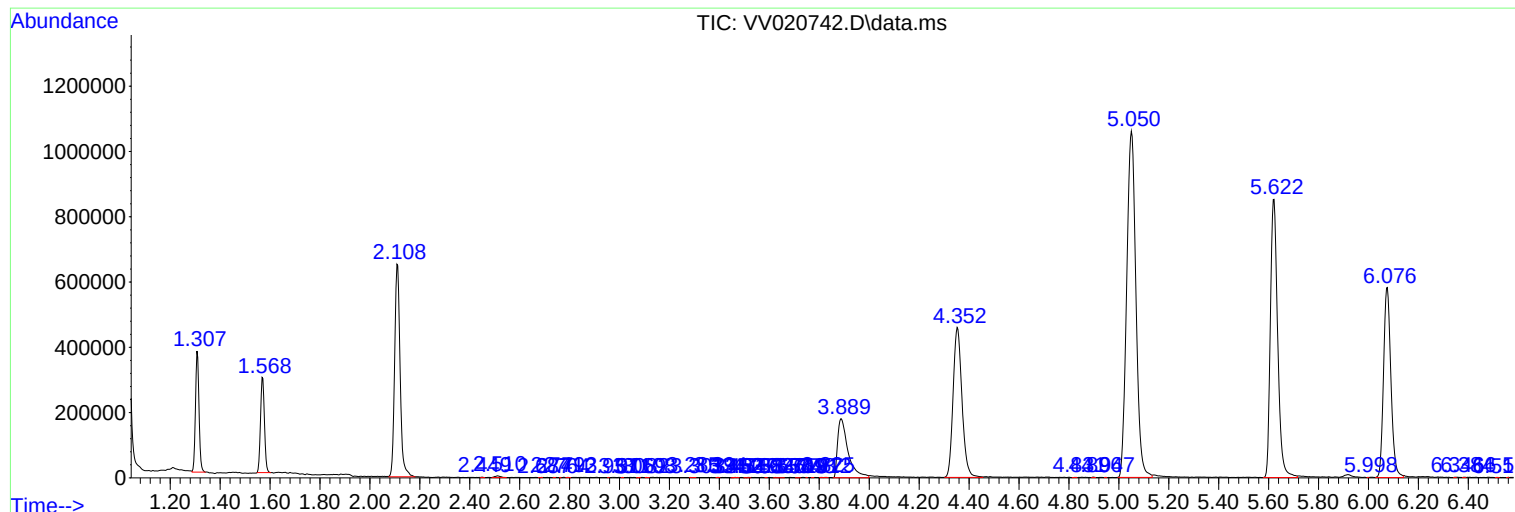

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020742.D
Acq On : 24 Mar 2021 17:15
Operator : SY/MD
Sample : M1783-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
Data File : VV020742.D
Acq On : 24 Mar 2021 17:15
Operator : SY/MD
Sample : M1783-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------