

m/z	Abundance
36.00	533.0
37.00	2767.0
38.10	2221.0
39.10	1028.0
40.00	256.0
44.00	953.0
45.00	572.0
45.80	113.0
46.30	122.0
47.20	819.0
48.00	465.0
49.10	2131.0
50.10	12071.0
51.10	3345.0
52.00	205.0
55.10	134.0
56.00	1177.0
57.00	1605.0
58.00	136.0
60.10	759.0
61.10	3189.0
62.10	3025.0
63.10	2583.0
64.10	423.0
65.10	648.0
67.00	142.0
68.10	6026.0
69.10	6700.0
70.00	510.0
71.90	313.0
72.30	274.0
73.10	3179.0
74.10	11684.0
75.10	33296.0
76.10	3056.0
76.90	206.0
77.40	223.0
78.10	112.0
79.00	2064.0
80.00	773.0
81.00	1881.0
81.90	525.0
83.30	128.0
86.10	109.0
87.00	2143.0
88.00	2435.0
91.10	240.0
92.00	1911.0
93.10	2565.0
94.10	8207.0
95.10	65088.0
96.10	4533.0
96.90	207.0
98.10	139.0
103.90	263.0
105.80	197.0
106.10	209.0
112.00	130.0
113.00	137.0
114.90	122.0
115.80	130.0
116.90	530.0
118.00	371.0
118.80	412.0
128.00	193.0
128.80	117.0
130.00	238.0
131.10	229.0
137.00	167.0
140.90	705.0
142.10	167.0
143.00	1045.0
145.00	144.0
146.00	157.0
147.10	116.0
147.70	207.0
148.00	143.0
149.10	102.0
150.00	122.0
151.90	121.0
154.80	236.0
156.90	139.0
172.00	521.0
173.00	852.0
174.00	57168.0
175.10	4080.0
176.00	54992.0
177.00	3738.0
178.00	191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	492.0
37.10	2881.0
38.10	2118.0
39.10	848.0
40.00	294.0
44.10	763.0
45.00	556.0
45.80	157.0
47.10	820.0
48.00	476.0
49.10	2278.0
50.10	11907.0
51.10	3080.0
52.00	296.0
55.00	134.0
56.10	1150.0
57.10	1579.0
60.20	842.0
61.10	3197.0
62.10	2733.0
63.10	2542.0
64.10	376.0
65.10	602.0
67.00	143.0
68.10	5917.0
69.10	6501.0
70.00	635.0
71.90	279.0
73.00	3032.0
74.10	10846.0
75.10	32656.0
76.10	2975.0
76.90	249.0
77.30	239.0
78.10	145.0
79.00	1967.0
80.00	752.0
81.00	1948.0
82.00	541.0
83.30	193.0
87.00	2258.0
88.00	2436.0
91.10	279.0
92.10	1863.0
93.00	2303.0
94.10	7613.0
95.10	62536.0
96.10	4439.0
96.90	212.0
98.10	111.0
103.80	167.0
104.90	116.0
106.00	289.0
112.00	120.0
112.90	155.0
114.90	110.0
116.00	115.0
116.90	385.0
118.00	257.0
118.80	402.0
128.00	194.0
130.00	302.0
131.10	212.0
135.00	134.0
137.10	227.0
141.00	794.0
142.00	147.0
143.00	1032.0
145.00	119.0
146.00	177.0
147.70	132.0
148.10	140.0
149.10	143.0
150.00	132.0
151.90	135.0
154.80	187.0
156.90	110.0
172.00	477.0
173.00	961.0
174.00	52784.0
175.00	3922.0
176.00	50192.0
177.00	3470.0
178.00	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
40.00	362.0
44.00	514.0
44.80	115.0
57.10	147.0
59.30	104.0
65.70	142.0
126.30	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	522.0
37.00	2359.0
38.10	2111.0
39.00	1097.0
40.10	303.0
44.00	1080.0
45.10	623.0
46.30	170.0
47.10	748.0
47.90	404.0
49.10	1909.0
50.10	11090.0
51.10	3376.0
52.00	109.0
53.00	158.0
55.20	113.0
56.10	947.0
57.00	1521.0
58.10	138.0
60.10	568.0
61.10	2801.0
62.10	3054.0
63.10	2273.0
64.10	444.0
65.10	680.0
67.00	149.0
68.10	5939.0
69.10	6049.0
70.10	406.0
71.90	264.0
72.30	253.0
73.10	3063.0
74.10	11039.0
75.10	30728.0
76.10	2773.0
77.20	230.0
78.00	129.0
79.00	1971.0
80.00	680.0
81.00	1749.0
81.90	464.0
86.10	155.0
87.00	2079.0
88.00	2139.0
91.00	202.0
92.00	1851.0
93.10	2697.0
94.10	7636.0
95.10	60872.0
96.10	4106.0
97.10	202.0
98.10	103.0
100.70	105.0
104.00	378.0
105.70	149.0
106.20	157.0
112.10	126.0
113.10	119.0
115.80	152.0
116.90	592.0
117.90	442.0
118.90	361.0
128.00	177.0
128.80	113.0
129.90	236.0
131.10	146.0
133.80	102.0
136.90	139.0
140.90	628.0
142.00	181.0
143.00	919.0
144.00	119.0
145.00	167.0
145.90	159.0
147.70	204.0
149.90	104.0
154.90	277.0
156.90	116.0
158.70	107.0
171.90	580.0
173.10	712.0
174.00	55232.0
175.00	3855.0
176.00	53216.0
177.00	3533.0
178.00	134.0



Instrument :
MSVOA_V
ClientSampleId :
BFB71

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032421\
 Data File : VV020722.D
 Acq On : 24 Mar 2021 08:26
 Operator : SY/MD
 Sample : BFB68
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB71

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis
 Last Update : Thu Mar 25 03:10:36 2021

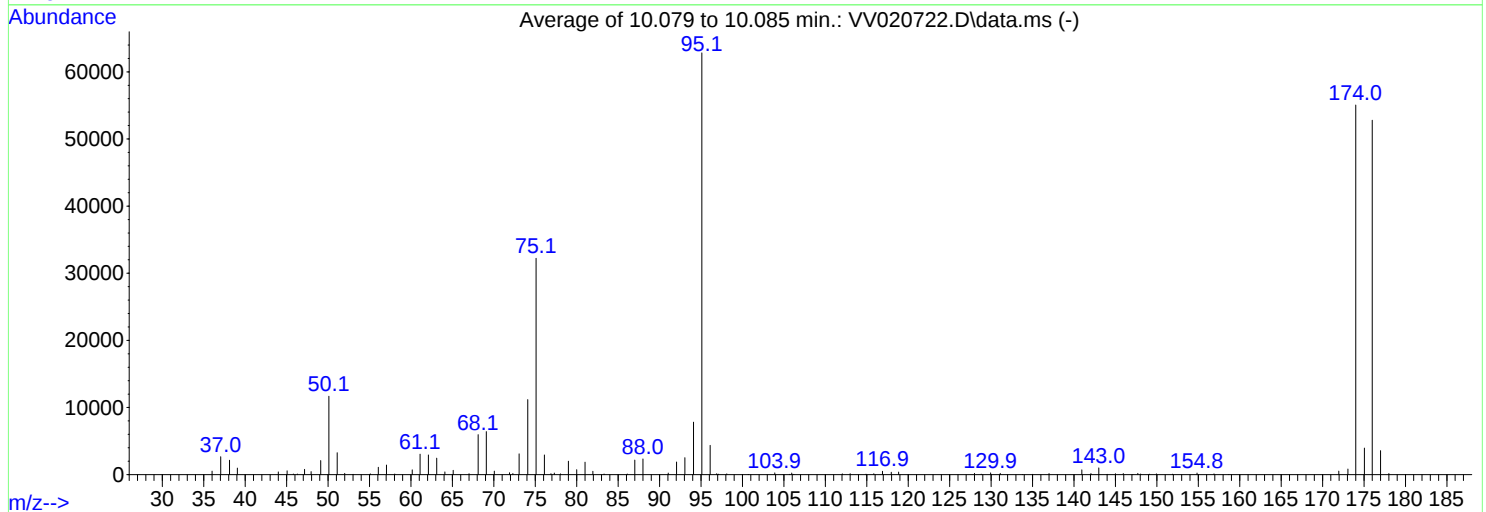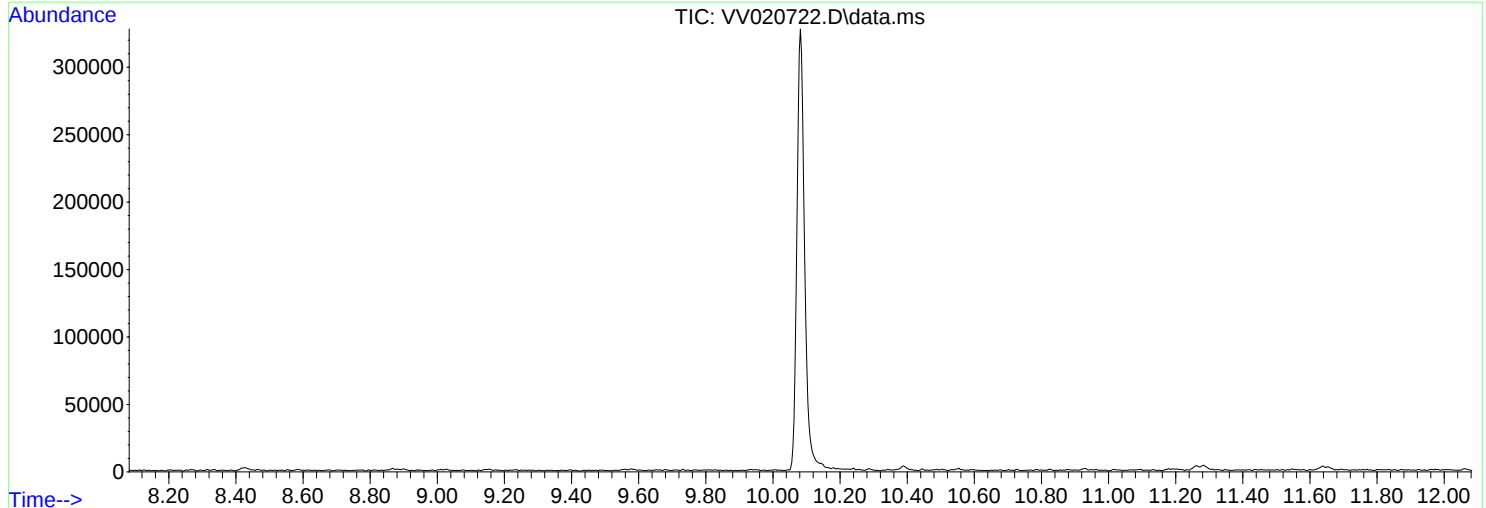

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	11689	PASS
75	95	30	80	51.3	32227	PASS
95	95	100	100	100.0	62832	PASS
96	95	5	9	6.9	4359	PASS
173	174	0.00	2	1.5	842	PASS
174	95	50	120	87.6	55061	PASS
175	174	5	9	7.2	3952	PASS
176	174	95	101	95.9	52800	PASS
177	176	5	9	6.8	3580	PASS