

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
 Data File : VV025162.D
 Acq On : 24 Mar 2022 20:03
 Operator : SY/MD
 Sample : N2100-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF9

Quant Time: Mar 25 03:12:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 25 02:51:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	143583	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	137502	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61970	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42592	3.757	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.200%
7) Chloroethane-d5	1.571	69	40452	4.873	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.400%
11) 1,1-Dichloroethene-d2	2.111	63	58660	3.202	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.000%
20) 2-Butanone-d5	3.899	46	101497	74.088	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	148.180%#
24) Chloroform-d	4.352	84	97391	5.180	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.600%
26) 1,2-Dichloroethane-d4	5.037	65	43750	5.566	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.400%
32) Benzene-d6	5.053	84	193899	4.861	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
36) 1,2-Dichloropropane-d6	6.069	67	59613	5.197	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.000%
41) Toluene-d8	7.317	98	160021	4.402	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.000%
43) trans-1,3-Dichloroprop...	7.629	79	17041	4.262	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.200%
46) 2-Hexanone-d5	8.088	63	80209	58.809	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	117.620%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	38990	5.778	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	57975	5.526	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.600%
Target Compounds						
25) Chloroform	4.388	83	2274	0.117	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025162.D
Acq On : 24 Mar 2022 20:03
Operator : SY/MD
Sample : N2100-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9

Quant Time: Mar 25 03:12:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 25 02:51:12 2022
Response via : Initial Calibration

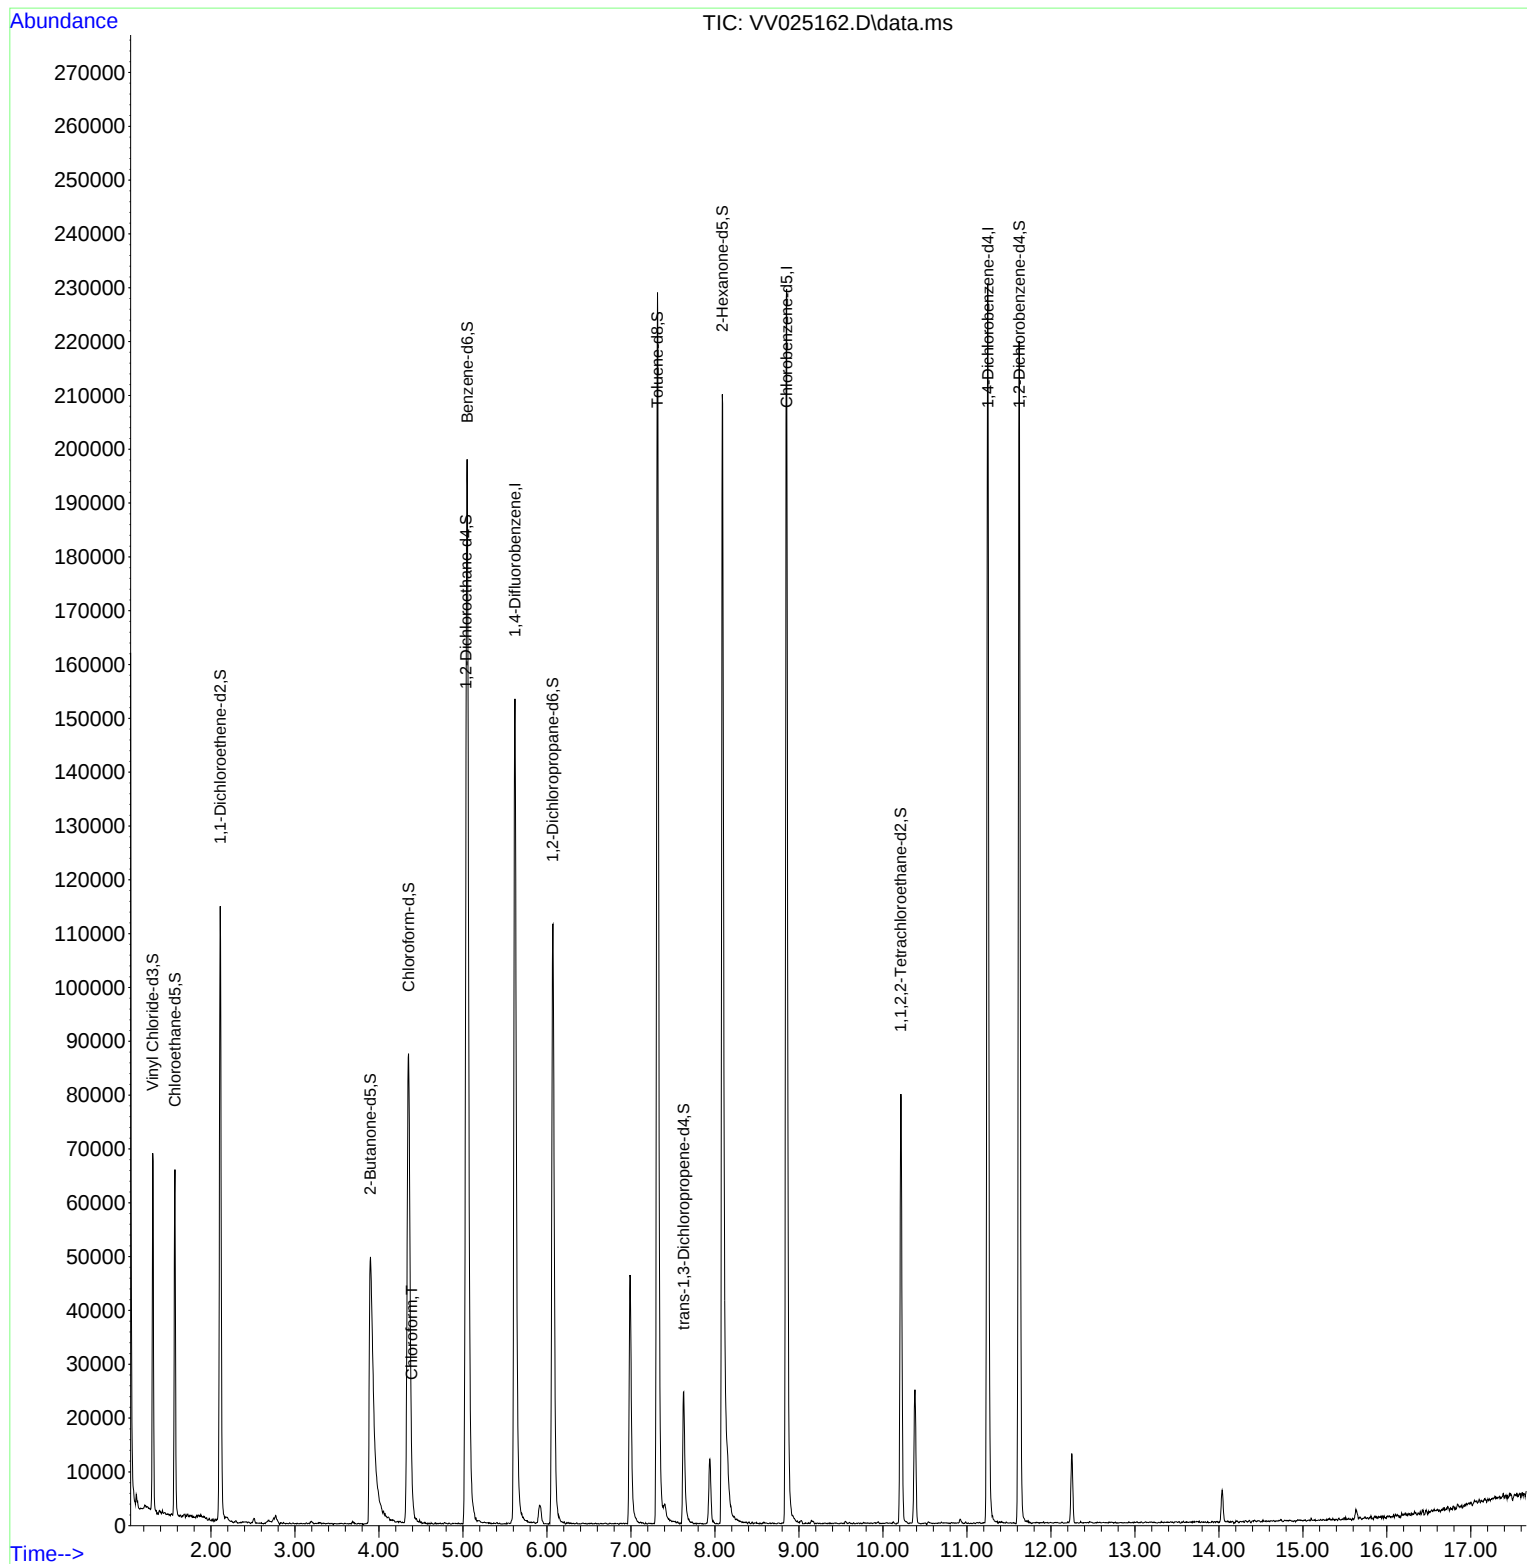

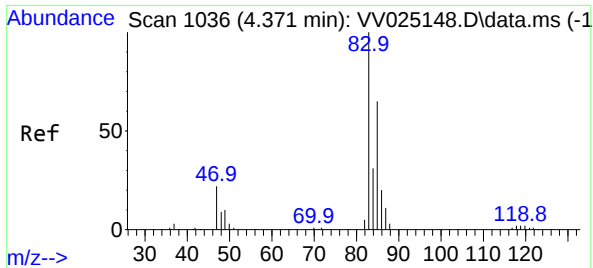

#25
Chloroform
Concen: 0.117 ug/L
RT: 4.388 min Scan# 10
Delta R.T. 0.016 min
Lab File: VV025162.D
Acq: 24 Mar 2022 20:03

Instrument :
MSVOA_V
ClientSampleId :
C0AF9

Tgt Ion: 83 Resp: 2274
Ion Ratio Lower Upper
83 100
85 64.2 44.5 82.7

