

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
 Data File : VV025154.D
 Acq On : 24 Mar 2022 16:56
 Operator : SY/MD
 Sample : N2100-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	100	rVB	67453	69548	14.38%	1.644%
2	1.571	157	165	175	rBV	62948	70185	14.51%	1.659%
3	1.754	216	222	232	rVB2	4658	6025	1.25%	0.142%
4	2.111	322	333	352	rVB	114399	165249	34.17%	3.907%
5	2.770	524	538	557	rBV	53747	112201	23.20%	2.653%
6	3.198	654	671	687	rVB2	7246	15757	3.26%	0.373%
7	3.896	878	888	931	rBV	49308	167728	34.68%	3.965%
8	4.352	1013	1030	1069	rVB2	90236	250041	51.70%	5.911%
9	5.050	1231	1247	1277	rBV2	192283	483614	100.00%	11.434%
10	5.619	1412	1424	1456	rBV	169909	350106	72.39%	8.277%
11	6.069	1550	1564	1590	rBV	109285	228884	47.33%	5.411%
12	6.989	1840	1850	1876	rBV	45442	86582	17.90%	2.047%
13	7.317	1940	1952	1974	rBV	229455	405415	83.83%	9.585%
14	7.625	2037	2048	2069	rBV	24807	45843	9.48%	1.084%
15	7.940	2133	2146	2154	rBV3	9319	15389	3.18%	0.364%
16	8.088	2183	2192	2237	rBV	203125	401813	83.09%	9.500%
17	8.850	2419	2429	2456	rBV	253158	420988	87.05%	9.953%
18	10.214	2842	2853	2875	rBV	78438	124416	25.73%	2.941%
19	10.381	2894	2905	2919	rVB2	20018	32221	6.66%	0.762%
20	11.246	3164	3174	3200	rBV	250248	396206	81.93%	9.367%
21	11.622	3280	3291	3311	rBV	222258	347970	71.95%	8.227%
22	12.249	3474	3486	3497	rVB2	9662	16291	3.37%	0.385%
23	14.040	4031	4043	4054	rVB	10445	17310	3.58%	0.409%




Sum of corrected areas: 4229782

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025154.D
Acq On : 24 Mar 2022 16:56
Operator : SY/MD
Sample : N2100-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

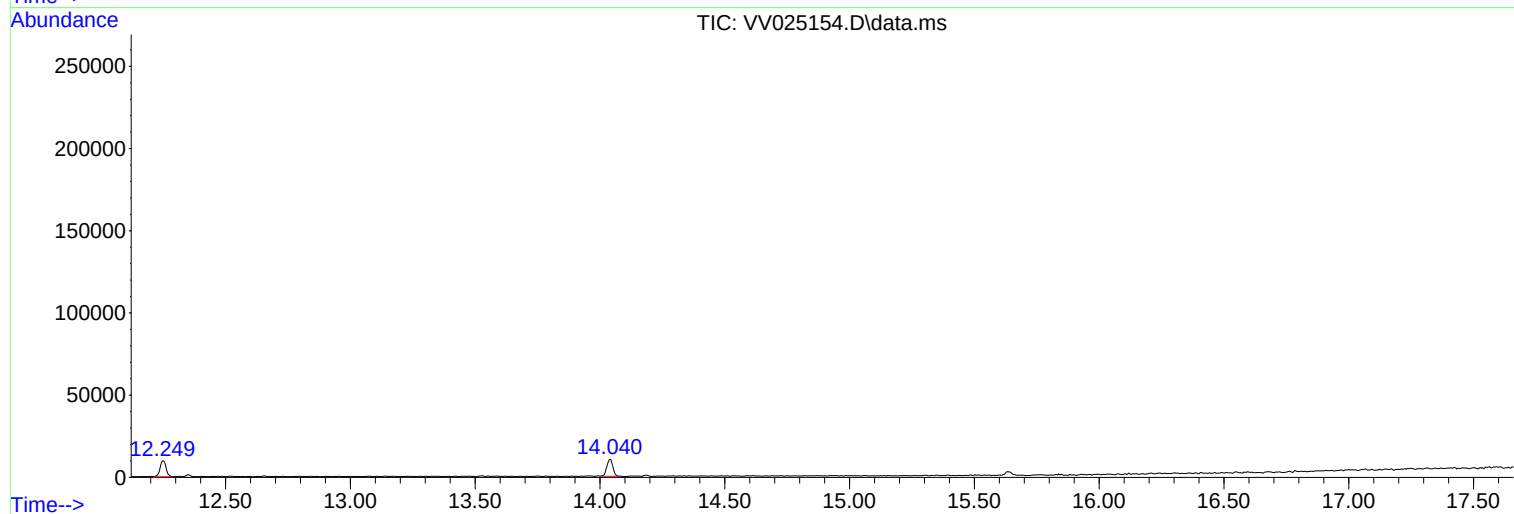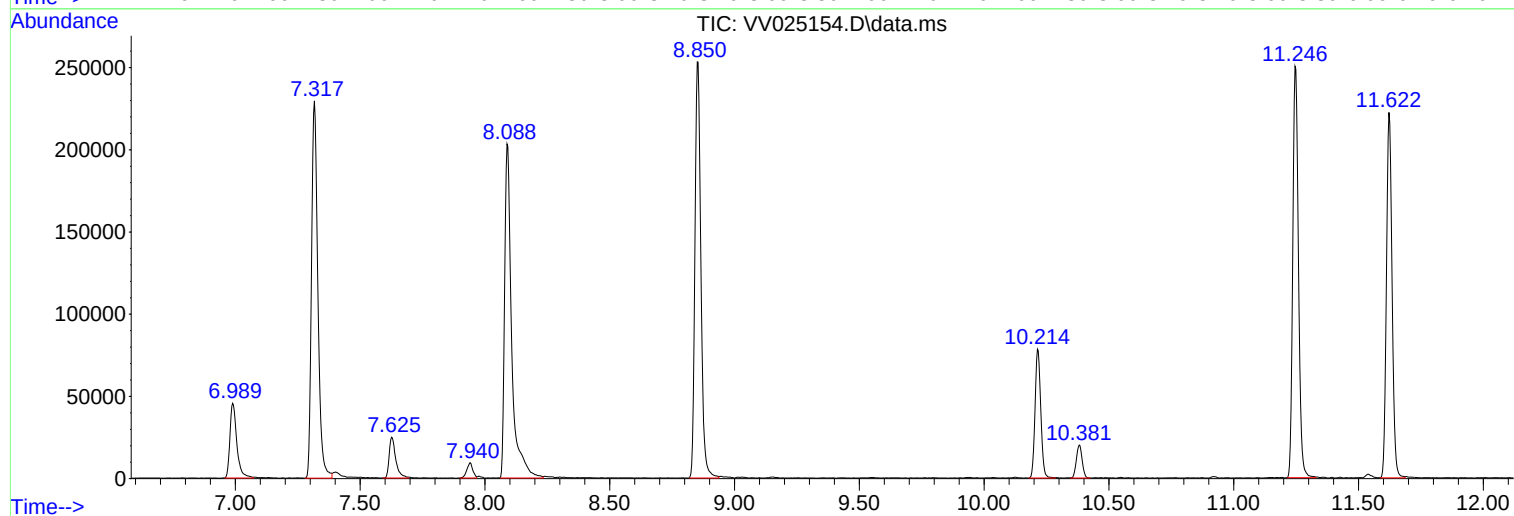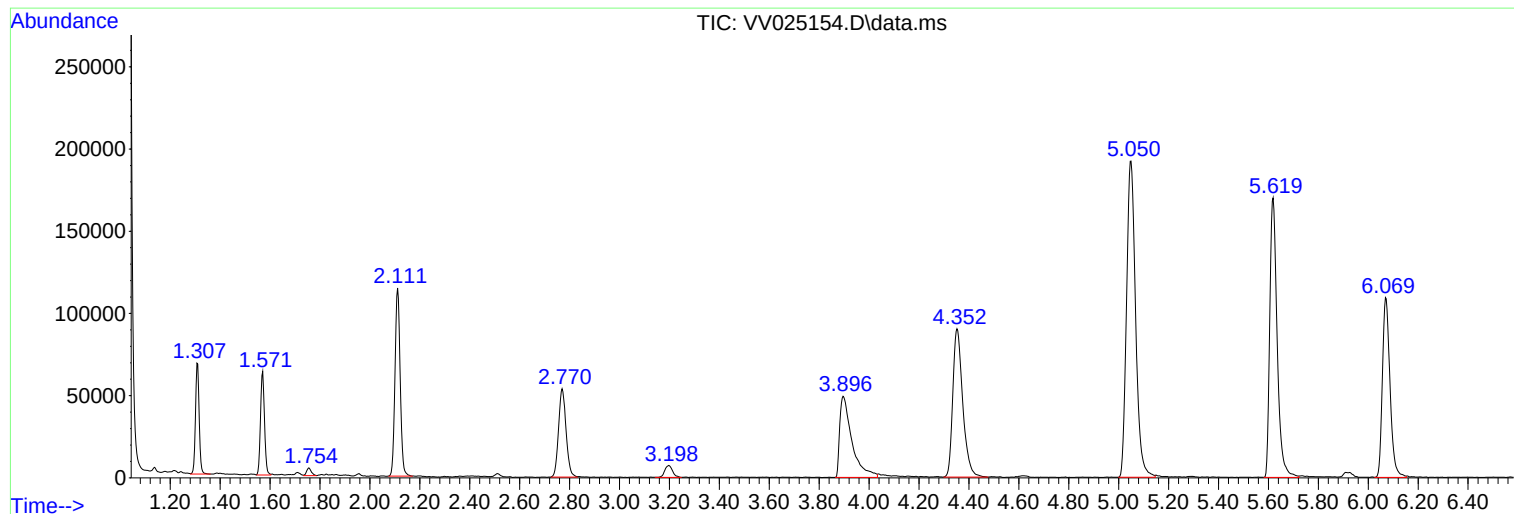

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025154.D
Acq On : 24 Mar 2022 16:56
Operator : SY/MD
Sample : N2100-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025154.D
Acq On : 24 Mar 2022 16:56
Operator : SY/MD
Sample : N2100-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc