

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
 Data File : VV025155.D
 Acq On : 24 Mar 2022 17:19
 Operator : SY/MD
 Sample : N2100-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	107916	110260	17.08%	2.254%
2	1.571	156	165	181	rBV	86873	98683	15.28%	2.017%
3	2.111	322	333	351	rBV	175953	252772	39.15%	5.168%
4	2.773	525	539	559	rVB3	3861	8640	1.34%	0.177%
5	3.899	878	889	923	rBV	51367	178018	27.57%	3.639%
6	4.352	1014	1030	1066	rBV2	113036	302701	46.88%	6.188%
7	5.050	1231	1247	1279	rBV2	261489	645722	100.00%	13.201%
8	5.619	1413	1424	1451	rBV	158201	322982	50.02%	6.603%
9	6.069	1550	1564	1595	rBV	141846	291229	45.10%	5.954%
10	6.989	1840	1850	1879	rBV	61791	114376	17.71%	2.338%
11	7.317	1940	1952	1971	rBV	325071	568479	88.04%	11.622%
12	7.400	1972	1978	1995	rVB3	5085	10886	1.69%	0.223%
13	7.625	2038	2048	2069	rBV	33754	61052	9.45%	1.248%
14	7.940	2134	2146	2151	rBV2	10375	18402	2.85%	0.376%
15	7.979	2151	2158	2174	rVB2	28332	49015	7.59%	1.002%
16	8.088	2183	2192	2226	rBV	225887	440378	68.20%	9.003%
17	8.853	2418	2430	2457	rBV	232439	394488	61.09%	8.065%
18	10.217	2842	2854	2874	rBV	90271	142412	22.05%	2.911%
19	10.381	2895	2905	2917	rVB2	23752	38049	5.89%	0.778%
20	11.249	3163	3175	3194	rBV	241821	372880	57.75%	7.623%
21	11.622	3279	3291	3313	rBV	287900	445881	69.05%	9.116%
22	12.252	3472	3487	3497	rBV	9542	15780	2.44%	0.323%
23	14.040	4033	4043	4053	rVB	5210	8287	1.28%	0.169%




Sum of corrected areas: 4891372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025155.D
Acq On : 24 Mar 2022 17:19
Operator : SY/MD
Sample : N2100-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

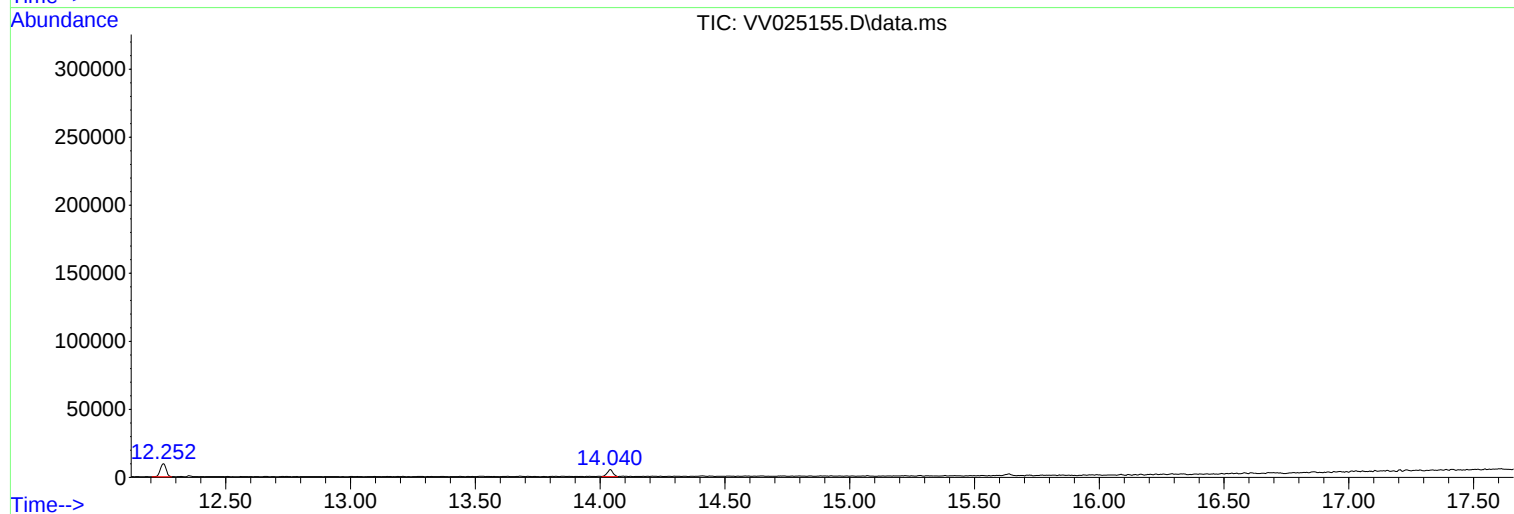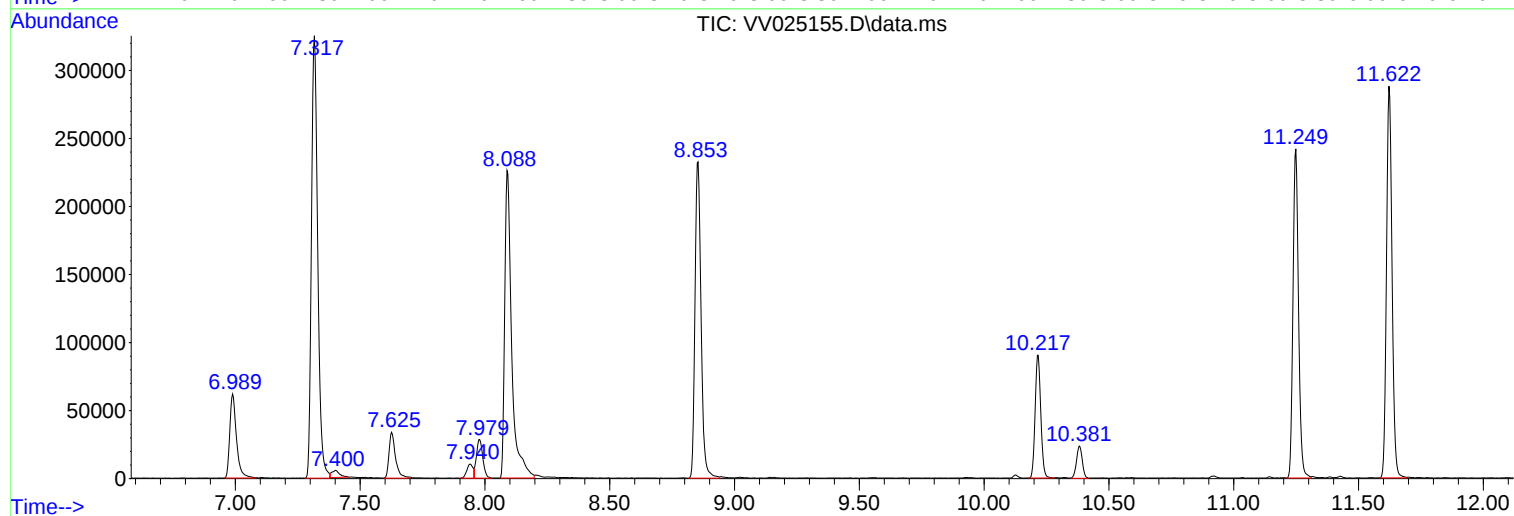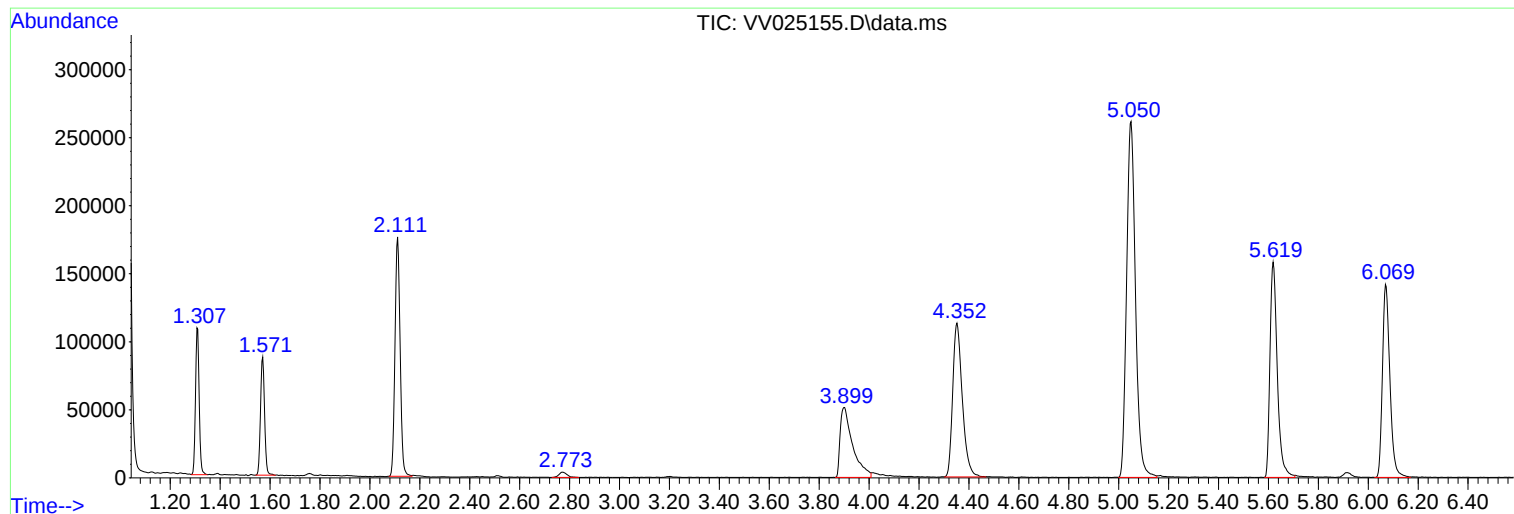

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025155.D
Acq On : 24 Mar 2022 17:19
Operator : SY/MD
Sample : N2100-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025155.D
Acq On : 24 Mar 2022 17:19
Operator : SY/MD
Sample : N2100-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc