

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
 Data File : VV025158.D
 Acq On : 24 Mar 2022 18:30
 Operator : SY/MD
 Sample : N2100-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	102	rVB	108175	111178	17.37%	2.377%
2	1.571	156	165	181	rBV	86741	97307	15.20%	2.081%
3	2.111	322	333	351	rBV	173173	249675	39.00%	5.339%
4	2.773	524	539	552	rBV3	5952	11779	1.84%	0.252%
5	3.899	878	889	932	rBV	49161	172628	26.96%	3.692%
6	4.352	1014	1030	1060	rBV2	110856	290656	45.40%	6.216%
7	5.050	1229	1247	1277	rBV2	257191	640227	100.00%	13.691%
8	5.619	1410	1424	1457	rBV	143901	298008	46.55%	6.373%
9	5.915	1507	1516	1533	rVB6	3595	7670	1.20%	0.164%
10	6.069	1551	1564	1588	rBV2	140318	286498	44.75%	6.127%
11	6.989	1835	1850	1875	rBV	60470	113088	17.66%	2.418%
12	7.317	1939	1952	1972	rBV	319306	558880	87.29%	11.951%
13	7.400	1975	1978	1991	rVB	4193	6473	1.01%	0.138%
14	7.625	2039	2048	2070	rBV	32762	59858	9.35%	1.280%
15	7.940	2134	2146	2160	rBV3	8915	15802	2.47%	0.338%
16	8.088	2183	2192	2230	rBV	225452	433944	67.78%	9.280%
17	8.853	2419	2430	2454	rBV	215044	360588	56.32%	7.711%
18	10.217	2843	2854	2876	rVB	88149	138759	21.67%	2.967%
19	10.381	2893	2905	2917	rBV	20614	32210	5.03%	0.689%
20	11.249	3164	3175	3193	rBV	214224	334948	52.32%	7.163%
21	11.622	3279	3291	3316	rBV	279129	435349	68.00%	9.310%
22	12.249	3475	3486	3497	rVB2	8424	13688	2.14%	0.293%
23	14.037	4031	4042	4053	rVB	4327	7088	1.11%	0.152%




Sum of corrected areas: 4676301

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025158.D
Acq On : 24 Mar 2022 18:30
Operator : SY/MD
Sample : N2100-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

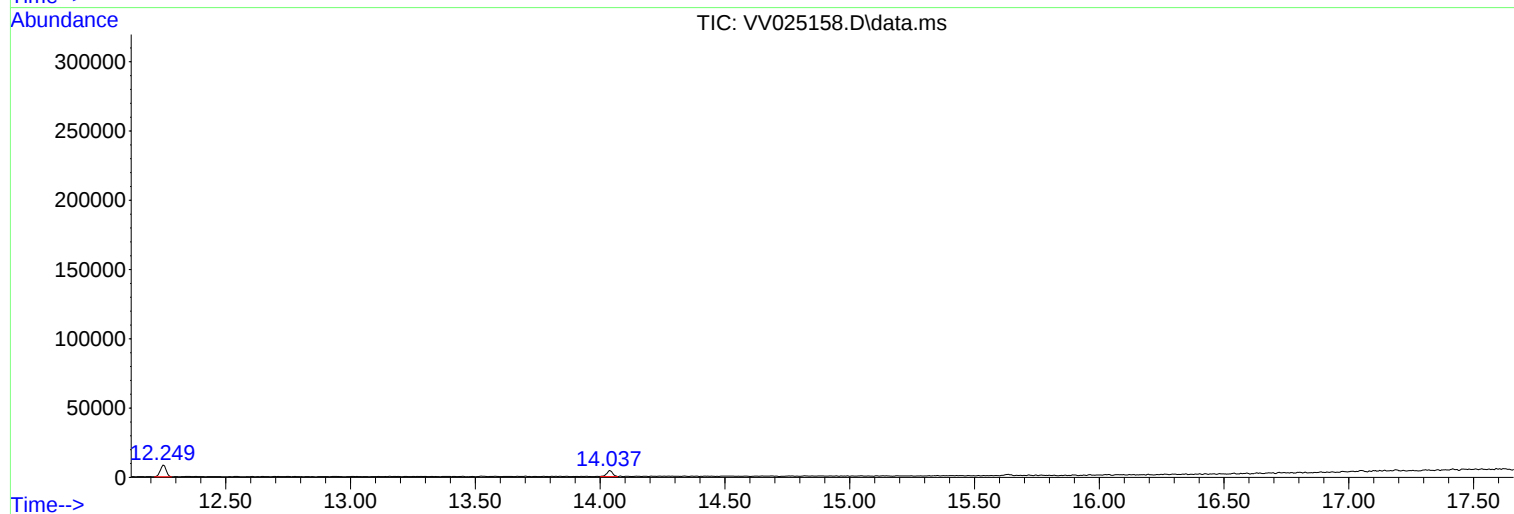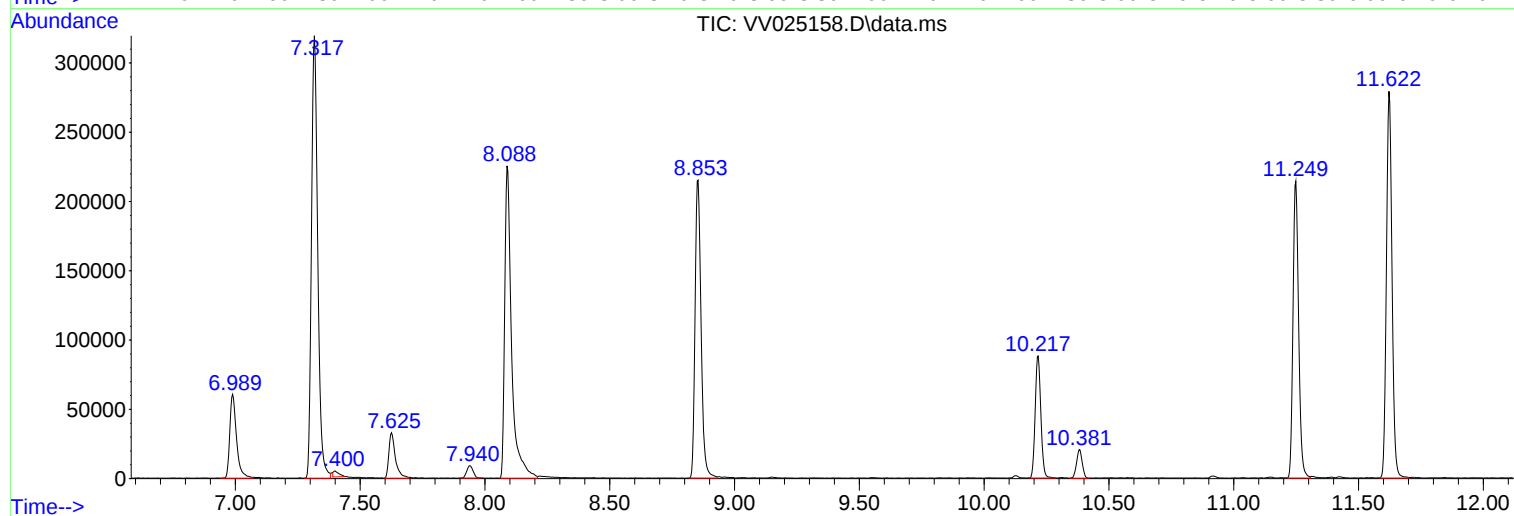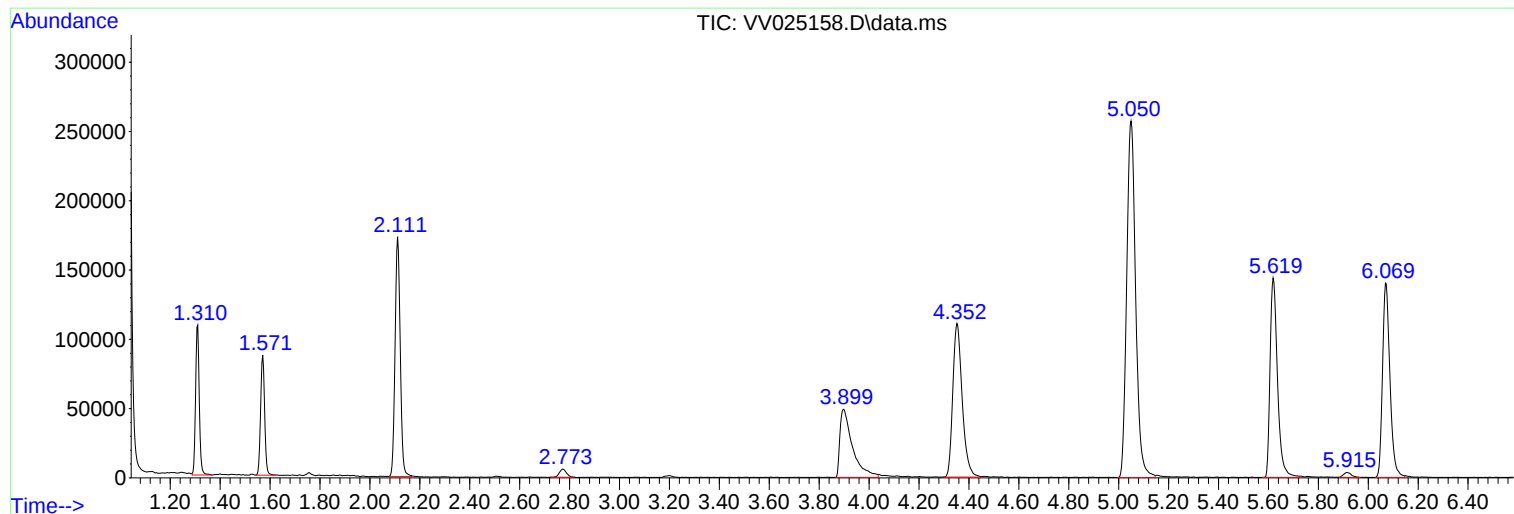

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025158.D
Acq On : 24 Mar 2022 18:30
Operator : SY/MD
Sample : N2100-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025158.D
Acq On : 24 Mar 2022 18:30
Operator : SY/MD
Sample : N2100-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc