

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
 Data File : VV025161.D
 Acq On : 24 Mar 2022 19:40
 Operator : SY/MD
 Sample : N2100-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	68293	68759	13.86%	1.679%
2	1.571	157	165	179	rVB	63500	71948	14.50%	1.757%
3	1.937	273	279	288	rVB3	4819	7051	1.42%	0.172%
4	2.111	322	333	351	rBV	116782	168744	34.02%	4.120%
5	2.510	449	457	468	rVB3	4713	8075	1.63%	0.197%
6	3.902	880	890	930	rBV	44746	169653	34.20%	4.143%
7	4.355	1013	1031	1060	rBV3	103297	332685	67.07%	8.123%
8	5.050	1231	1247	1281	rBV2	200620	496042	100.00%	12.112%
9	5.619	1411	1424	1462	rBV	144987	298567	60.19%	7.290%
10	5.911	1506	1515	1531	rVB5	4502	10090	2.03%	0.246%
11	6.072	1552	1565	1598	rBV	113648	238154	48.01%	5.815%
12	6.989	1841	1850	1877	rBV	46577	88707	17.88%	2.166%
13	7.317	1941	1952	1971	rBV	229059	406424	81.93%	9.924%
14	7.397	1972	1977	1990	rVB4	4272	8717	1.76%	0.213%
15	7.625	2039	2048	2067	rBV	24420	45514	9.18%	1.111%
16	7.940	2132	2146	2158	rBV3	12038	22304	4.50%	0.545%
17	8.091	2182	2193	2237	rBV	210153	423340	85.34%	10.337%
18	8.854	2419	2430	2459	rBV	218099	361198	72.82%	8.820%
19	10.217	2843	2854	2868	rBV	79575	124912	25.18%	3.050%
20	10.381	2893	2905	2919	rBV	28683	46018	9.28%	1.124%
21	11.249	3158	3175	3196	rBV	213244	332517	67.03%	8.119%
22	11.622	3280	3291	3314	rBV	222593	350652	70.69%	8.562%
23	12.249	3476	3486	3497	rVB2	10163	15352	3.09%	0.375%


Sum of corrected areas: 4095423

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025161.D
Acq On : 24 Mar 2022 19:40
Operator : SY/MD
Sample : N2100-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

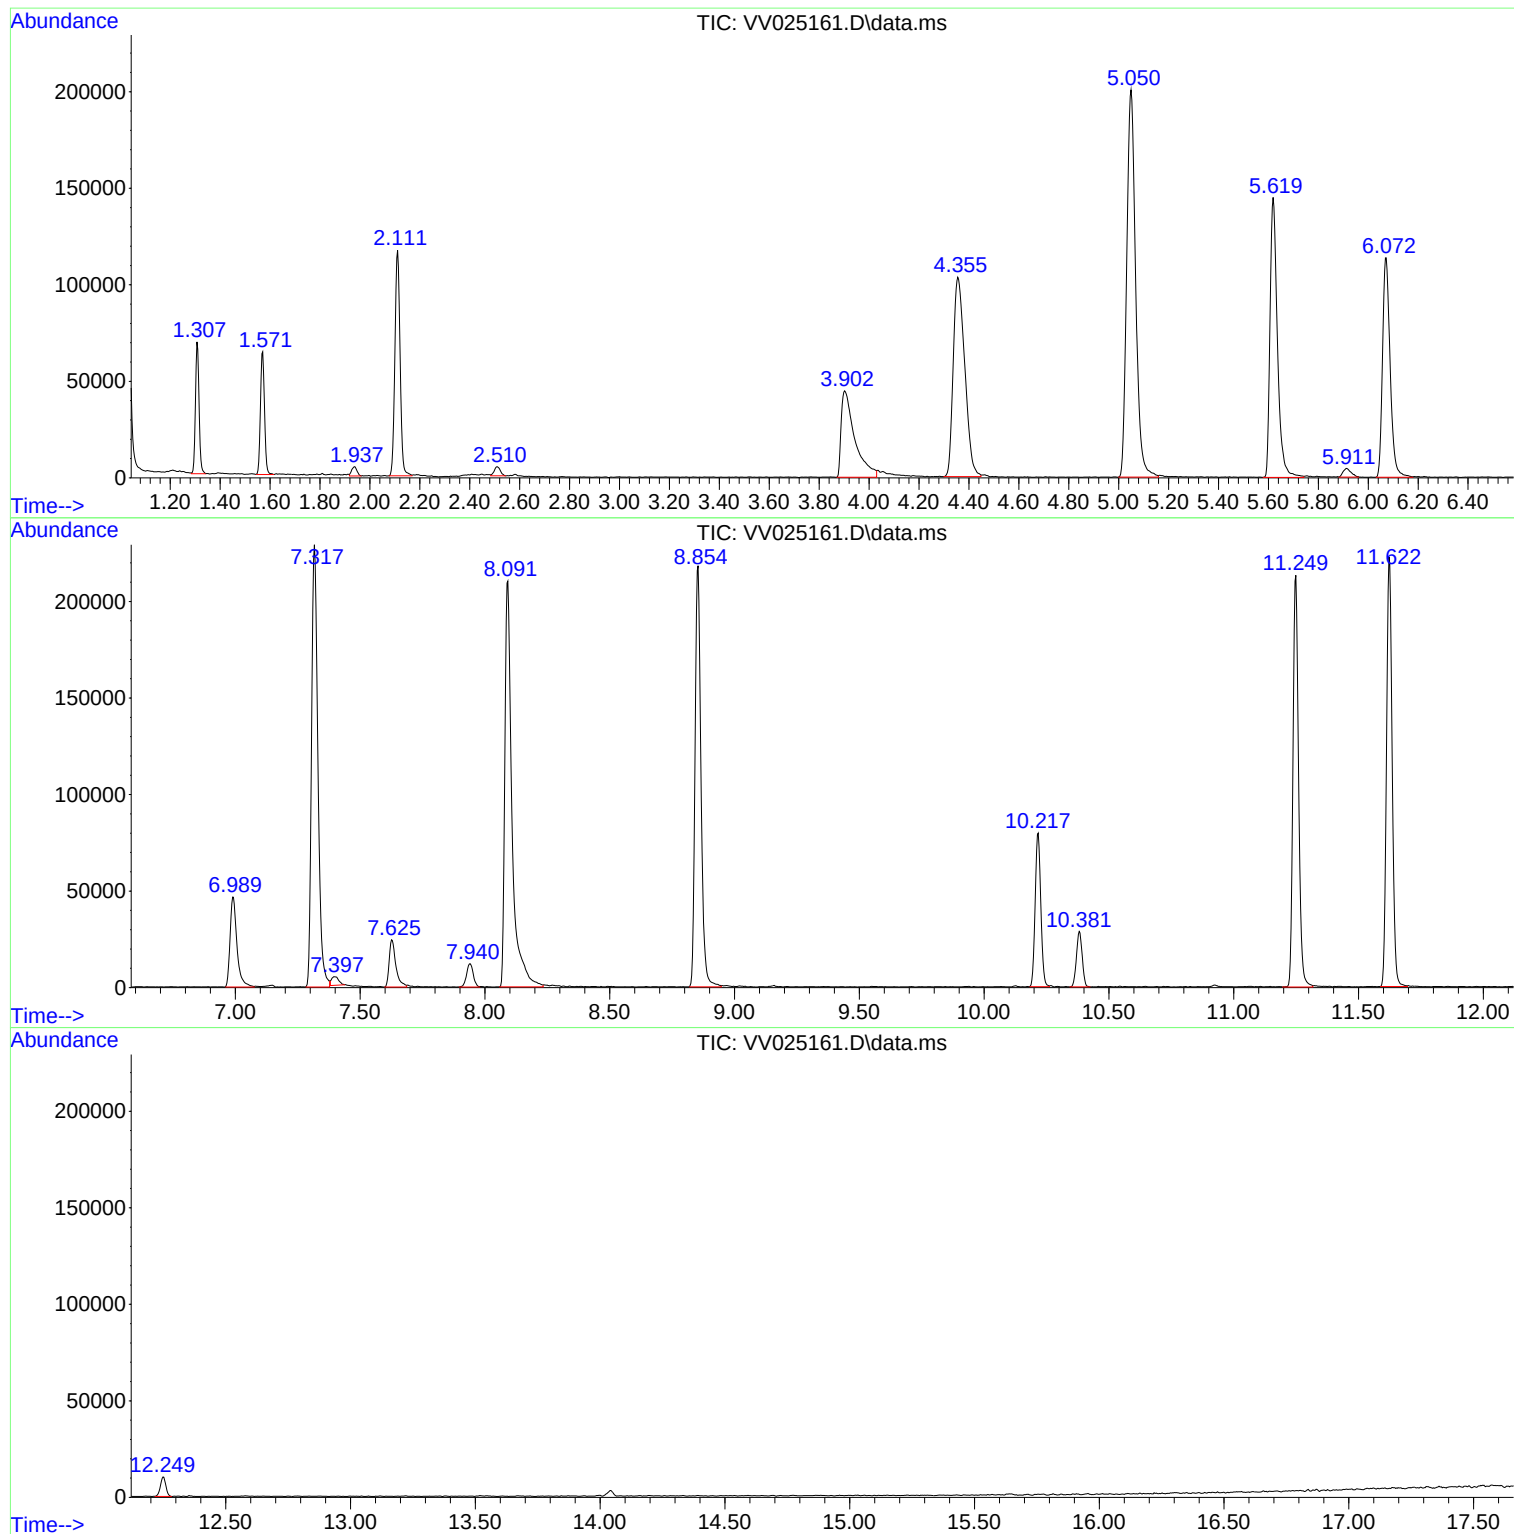

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025161.D
Acq On : 24 Mar 2022 19:40
Operator : SY/MD
Sample : N2100-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025161.D
Acq On : 24 Mar 2022 19:40
Operator : SY/MD
Sample : N2100-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc