

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
 Data File : VV025162.D
 Acq On : 24 Mar 2022 20:03
 Operator : SY/MD
 Sample : N2100-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	66432	67942	13.81%	1.703%
2	1.571	156	165	181	rVB	64453	71027	14.44%	1.781%
3	2.111	323	333	349	rBV	113873	164041	33.35%	4.112%
4	3.899	878	889	934	rBV2	49492	181690	36.94%	4.555%
5	4.352	1014	1030	1057	rBV2	87110	221776	45.09%	5.560%
6	5.050	1231	1247	1277	rBV2	197811	491811	100.00%	12.329%
7	5.619	1409	1424	1448	rBV	153151	315882	64.23%	7.919%
8	5.912	1507	1515	1531	rVB6	3430	7948	1.62%	0.199%
9	6.072	1553	1565	1585	rBV	111395	230464	46.86%	5.777%
10	6.989	1840	1850	1870	rBV	46251	85933	17.47%	2.154%
11	7.317	1940	1952	1971	rBV	228744	402189	81.78%	10.082%
12	7.629	2040	2049	2067	rBV	24450	44483	9.04%	1.115%
13	7.940	2135	2146	2157	rBV3	11933	20765	4.22%	0.521%
14	8.088	2183	2192	2222	rBV	209756	406439	82.64%	10.189%
15	8.854	2419	2430	2451	rBV	229276	381325	77.53%	9.559%
16	10.214	2842	2853	2872	rBV	79758	124748	25.37%	3.127%
17	10.381	2894	2905	2920	rVB	24822	40443	8.22%	1.014%
18	11.249	3164	3175	3191	rBV	230256	353176	71.81%	8.854%
19	11.622	3279	3291	3314	rBV	219728	347134	70.58%	8.702%
20	12.249	3475	3486	3497	rVB2	12923	20112	4.09%	0.504%
21	14.040	4033	4043	4057	rBV	5945	9771	1.99%	0.245%


Sum of corrected areas: 3989099

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025162.D
Acq On : 24 Mar 2022 20:03
Operator : SY/MD
Sample : N2100-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

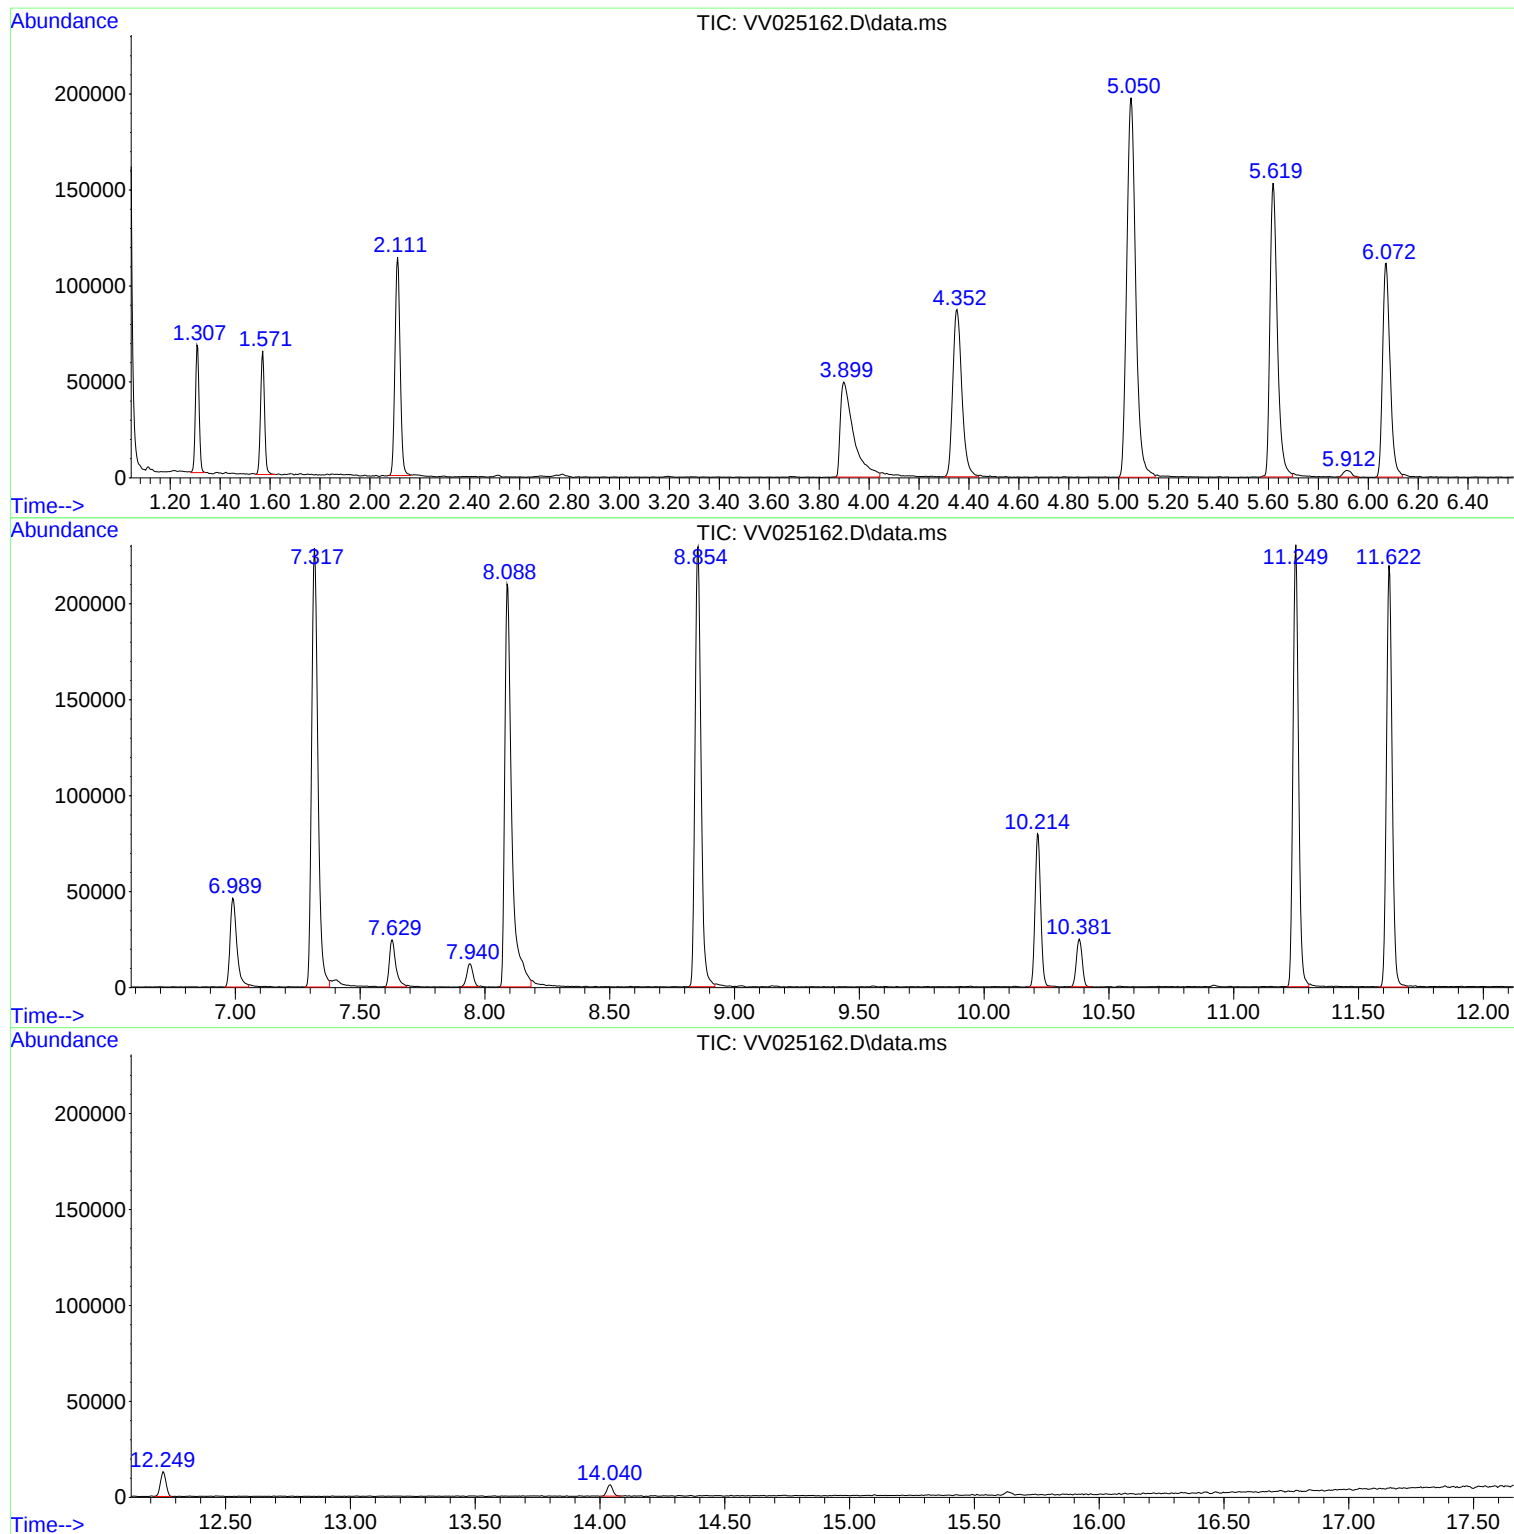

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025162.D
Acq On : 24 Mar 2022 20:03
Operator : SY/MD
Sample : N2100-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025162.D
Acq On : 24 Mar 2022 20:03
Operator : SY/MD
Sample : N2100-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc