

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
 Data File : VV025163.D
 Acq On : 24 Mar 2022 20:27
 Operator : SY/MD
 Sample : N2100-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	101	rVB	70955	72809	14.34%	1.755%
2	1.571	156	165	178	rBV	64440	73294	14.43%	1.767%
3	2.111	321	333	347	rBV	119300	171640	33.80%	4.138%
4	3.899	878	889	930	rBV2	50620	179370	35.32%	4.324%
5	4.352	1014	1030	1057	rBV	89791	228385	44.97%	5.506%
6	5.050	1231	1247	1273	rBV3	203690	507870	100.00%	12.243%
7	5.619	1409	1424	1453	rBV	145912	302154	59.49%	7.284%
8	5.915	1504	1516	1532	rVB7	3503	7963	1.57%	0.192%
9	6.072	1551	1565	1593	rBV	114910	242174	47.68%	5.838%
10	6.989	1841	1850	1871	rBV2	47333	90151	17.75%	2.173%
11	7.316	1940	1952	1973	rBV	237077	416478	82.00%	10.040%
12	7.625	2039	2048	2077	rBV	25844	47811	9.41%	1.153%
13	7.940	2133	2146	2157	rBV3	23566	43434	8.55%	1.047%
14	8.088	2183	2192	2231	rBV	218777	432208	85.10%	10.419%
15	8.853	2419	2430	2463	rBV	220684	369152	72.69%	8.899%
16	10.213	2841	2853	2875	rBV	84597	132129	26.02%	3.185%
17	10.381	2894	2905	2917	rBV2	50921	81219	15.99%	1.958%
18	11.249	3164	3175	3195	rBV	216425	337117	66.38%	8.127%
19	11.622	3277	3291	3313	rBV	232204	364662	71.80%	8.791%
20	12.249	3474	3486	3498	rBV2	22172	35283	6.95%	0.851%
21	14.040	4031	4043	4052	rBV	8161	12905	2.54%	0.311%


Sum of corrected areas: 4148208

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025163.D
Acq On : 24 Mar 2022 20:27
Operator : SY/MD
Sample : N2100-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

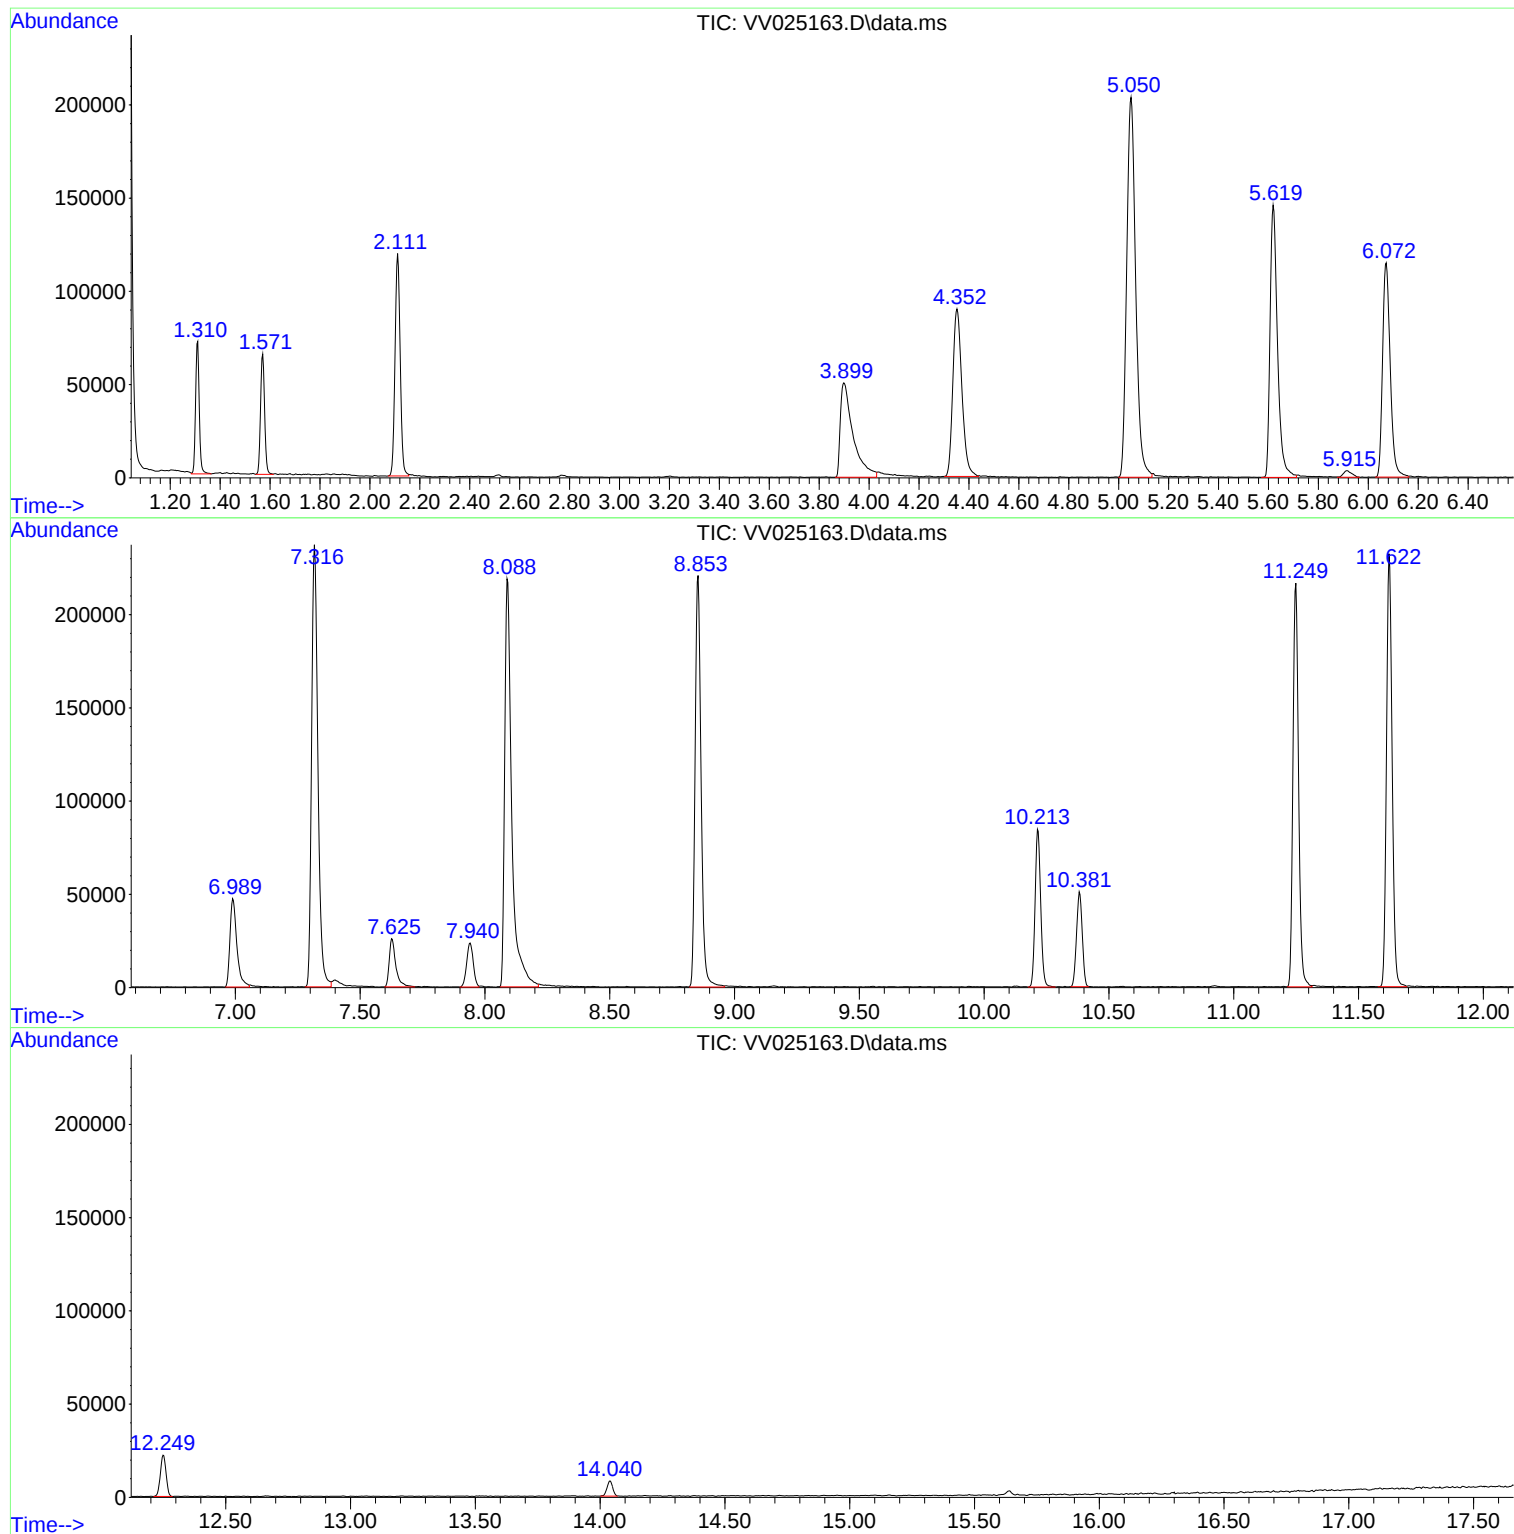

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025163.D
Acq On : 24 Mar 2022 20:27
Operator : SY/MD
Sample : N2100-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
Data File : VV025163.D
Acq On : 24 Mar 2022 20:27
Operator : SY/MD
Sample : N2100-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
