
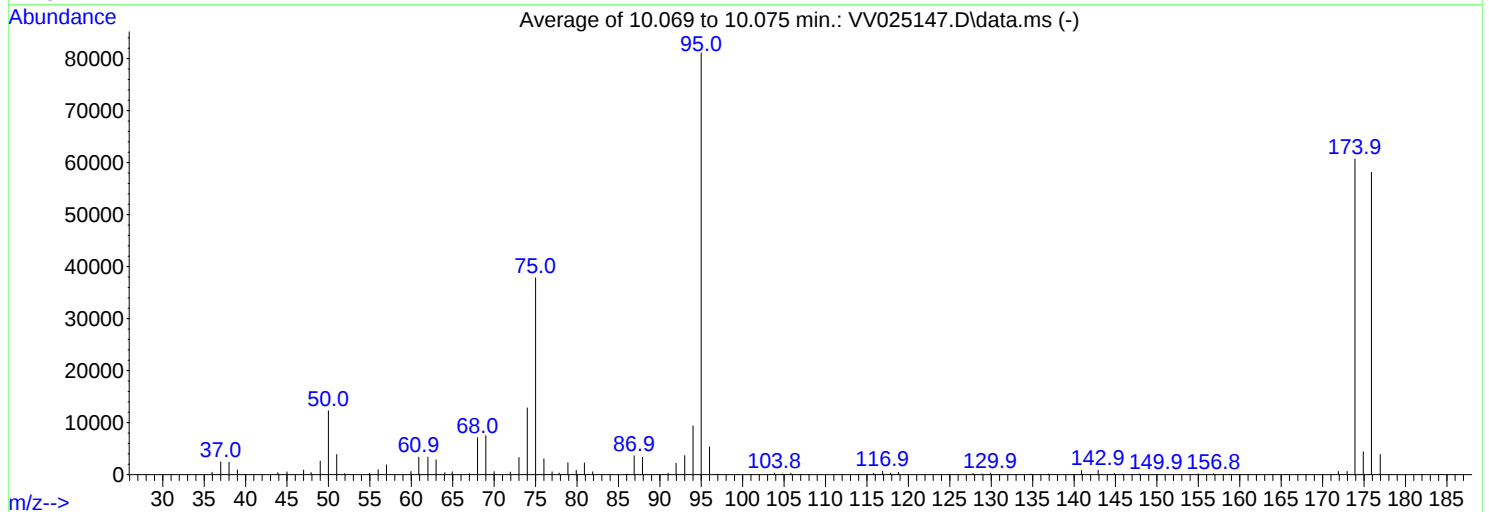


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032422\
 Data File : VV025147.D
 Acq On : 24 Mar 2022 11:04
 Operator : SY/MD
 Sample : BFB286
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB286

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 25 02:51:12 2022

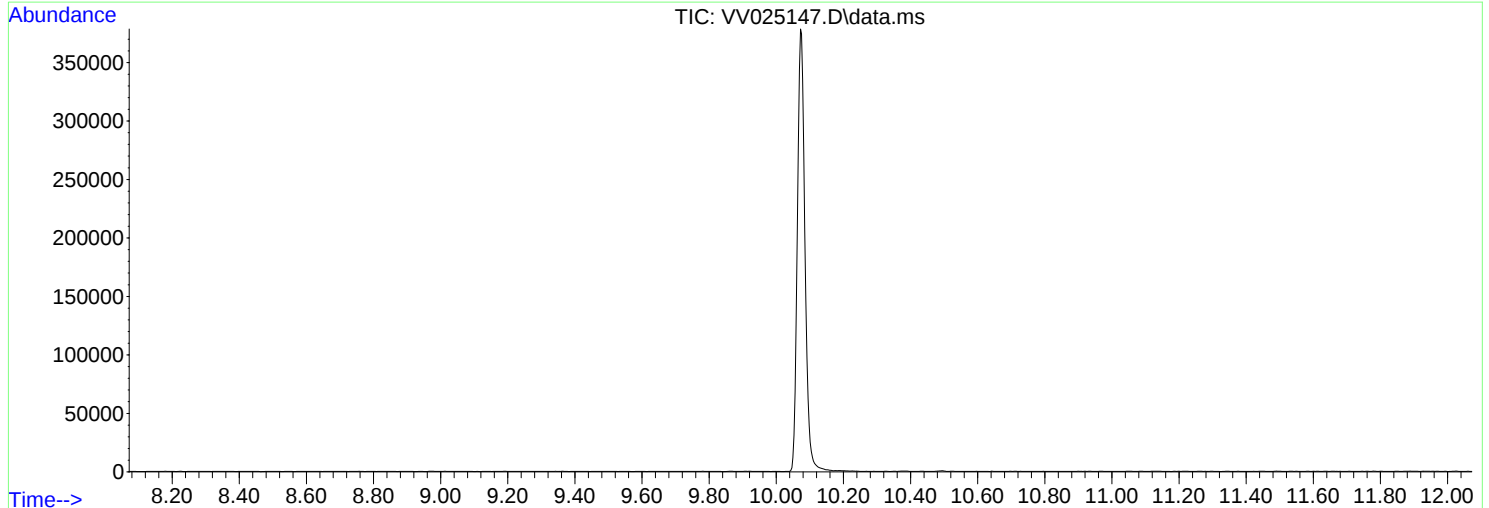

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	12289	PASS
75	95	30	80	46.7	37843	PASS
95	95	100	100	100.0	81101	PASS
96	95	5	9	6.6	5317	PASS
173	174	0.00	2	1.0	614	PASS
174	95	50	120	74.8	60680	PASS
175	174	5	9	7.3	4415	PASS
176	174	95	105	95.8	58123	PASS
177	176	5	10	6.7	3867	PASS

m/z	Abundance
40.00	143.0
43.90	274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
36.00	478.0
37.00	2203.0
38.00	2208.0
39.00	870.0
39.90	221.0
43.90	631.0
45.00	509.0
47.00	963.0
48.00	409.0
49.00	2486.0
50.00	11804.0
51.00	3859.0
52.00	188.0
54.90	241.0
56.00	900.0
57.00	1813.0
59.90	586.0
60.90	3344.0
62.00	3258.0
63.00	2650.0
64.10	408.0
65.00	552.0
67.00	153.0
68.00	6725.0
69.00	7024.0
70.00	518.0
72.00	507.0
73.00	3057.0
74.00	12354.0
75.00	35976.0
76.00	2916.0
77.00	499.0
77.80	301.0
78.90	2301.0
79.90	815.0
80.90	2119.0
81.90	524.0
86.10	136.0
86.90	3461.0
87.90	3176.0
91.00	266.0
91.90	2093.0
93.00	3458.0
94.00	9137.0
95.00	76176.0
96.00	5170.0
96.90	126.0
103.80	311.0
104.90	176.0
105.80	291.0
106.90	103.0
115.70	266.0
116.90	554.0
117.80	310.0
118.80	408.0
127.80	251.0
128.90	177.0
129.90	297.0
130.90	114.0
134.80	140.0
136.80	132.0
140.90	750.0
142.90	857.0
144.90	243.0
145.80	123.0
147.90	161.0
154.90	181.0
156.90	181.0
171.90	508.0
173.00	545.0
173.90	56000.0
174.90	4066.0
175.90	53240.0
176.90	3778.0
178.00	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
36.00	479.0
37.00	2550.0
38.00	2480.0
39.00	953.0
39.90	234.0
43.90	688.0
45.00	518.0
47.00	888.0
47.90	396.0
49.00	2694.0
50.00	12687.0
51.00	3967.0
51.90	214.0
54.90	249.0
56.00	976.0
57.00	1950.0
59.90	617.0
60.90	3442.0
62.00	3467.0
63.00	2934.0
64.10	445.0
64.90	567.0
67.00	195.0
68.00	7307.0
69.00	7765.0
70.00	623.0
72.00	527.0
73.00	3428.0
74.00	13330.0
75.00	39232.0
76.00	3138.0
77.00	569.0
77.80	319.0
78.90	2372.0
79.90	874.0
80.90	2331.0
81.90	578.0
86.00	141.0
86.90	3736.0
87.90	3430.0
91.00	313.0
91.90	2284.0
93.00	3868.0
94.00	9638.0
95.00	84352.0
96.00	5485.0
96.90	129.0
103.80	336.0
104.90	177.0
105.80	319.0
115.80	292.0
116.90	678.0
117.90	302.0
118.80	486.0
127.80	276.0
128.90	177.0
129.90	312.0
134.80	134.0
136.90	139.0
140.90	814.0
141.60	106.0
142.90	906.0
144.80	250.0
145.90	144.0
147.80	163.0
149.90	111.0
155.00	155.0
156.80	179.0
158.80	121.0
171.90	626.0
172.90	644.0
173.90	62664.0
174.90	4598.0
175.90	60216.0
176.90	3985.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
35.90	472.0
37.00	2681.0
38.00	2474.0
39.00	985.0
39.90	219.0
43.90	683.0
45.00	510.0
47.00	787.0
47.80	367.0
49.00	2677.0
50.00	12377.0
51.00	3793.0
51.90	208.0
55.00	218.0
56.00	981.0
57.00	1838.0
60.00	618.0
60.90	3259.0
62.00	3342.0
63.00	2936.0
64.00	380.0
64.90	520.0
67.00	212.0
68.00	7271.0
69.00	7724.0
70.00	647.0
71.90	462.0
73.00	3399.0
74.00	12854.0
75.00	38320.0
76.00	3095.0
77.00	566.0
77.90	324.0
78.90	2196.0
79.90	830.0
80.90	2319.0
81.90	571.0
86.10	133.0
86.90	3662.0
87.90	3413.0
91.00	326.0
92.00	2210.0
93.00	3680.0
94.00	9350.0
95.00	82776.0
96.00	5295.0
96.90	135.0
103.90	320.0
104.80	161.0
105.80	321.0
115.90	320.0
116.90	725.0
117.90	327.0
118.80	512.0
127.80	243.0
128.90	142.0
129.90	300.0
134.80	119.0
137.00	147.0
140.90	855.0
141.70	105.0
142.90	871.0
144.80	234.0
145.90	116.0
147.80	145.0
149.90	101.0
155.10	164.0
156.80	158.0
158.70	108.0
171.90	682.0
172.90	653.0
173.90	63376.0
174.90	4582.0
175.90	60912.0
177.00	3838.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
35.90	472.0
37.00	2681.0
38.00	2474.0
39.00	985.0
39.90	219.0
43.90	683.0
45.00	510.0
47.00	787.0
47.80	367.0
49.00	2677.0
50.00	12377.0
51.00	3793.0
51.90	208.0
55.00	218.0
56.00	981.0
57.00	1838.0
60.00	618.0
60.90	3259.0
62.00	3342.0
63.00	2936.0
64.00	380.0
64.90	520.0
67.00	212.0
68.00	7271.0
69.00	7724.0
70.00	647.0
71.90	462.0
73.00	3399.0
74.00	12854.0
75.00	38320.0
76.00	3095.0
77.00	566.0
77.90	324.0
78.90	2196.0
79.90	830.0
80.90	2319.0
81.90	571.0
86.10	133.0
86.90	3662.0
87.90	3413.0
91.00	326.0
92.00	2210.0
93.00	3680.0
94.00	9350.0
95.00	82776.0
96.00	5295.0
96.90	135.0
103.90	320.0
104.80	161.0
105.80	321.0
115.90	320.0
116.90	725.0
117.90	327.0
118.80	512.0
127.80	243.0
128.90	142.0
129.90	300.0
134.80	119.0
137.00	147.0
140.90	855.0
141.70	105.0
142.90	871.0
144.80	234.0
145.90	116.0
147.80	145.0
149.90	101.0
155.10	164.0
156.80	158.0
158.70	108.0
171.90	682.0
172.90	653.0
173.90	63376.0
174.90	4582.0
175.90	60912.0
177.00	3838.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286