

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV032425\
Data File : VV038737.D
Acq On : 24 Mar 2025 14:05
Operator : SY/MD
Sample : VV0324WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Mar 24 15:16:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM032425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Mar 24 15:12:15 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5585	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5293	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2420	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2500	0.48	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	96.00%
4) 1,2-Dichloroethane-d4	4.969	65	1307	0.49	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.00%
7) 1,2-Dichloropropane-d6	5.995	67	1509	0.46	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	92.00%
8) Toluene-d8	7.253	98	2913	0.48	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	96.00%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	1286	0.46	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	92.00%
Target Compounds						Qvalue
12) 1,2,3-Trichloropropane	10.214	75	45	0.02	ug/L #	71
13) 1,2-Dibromo-3-chloropr...	12.374	75	17	0.03	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

LABKSS
Client Sample ID :
MSVOA_V
Instrument :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV032425\
Data File : VV038737.D
Acq On : 24 Mar 2025 14:05
Operator : SY/MD
Sample : VV0324WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1





Quant Time: Mar 24 15:16:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM032425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Mar 24 15:12:15 2025
Response via : Initial Calibration

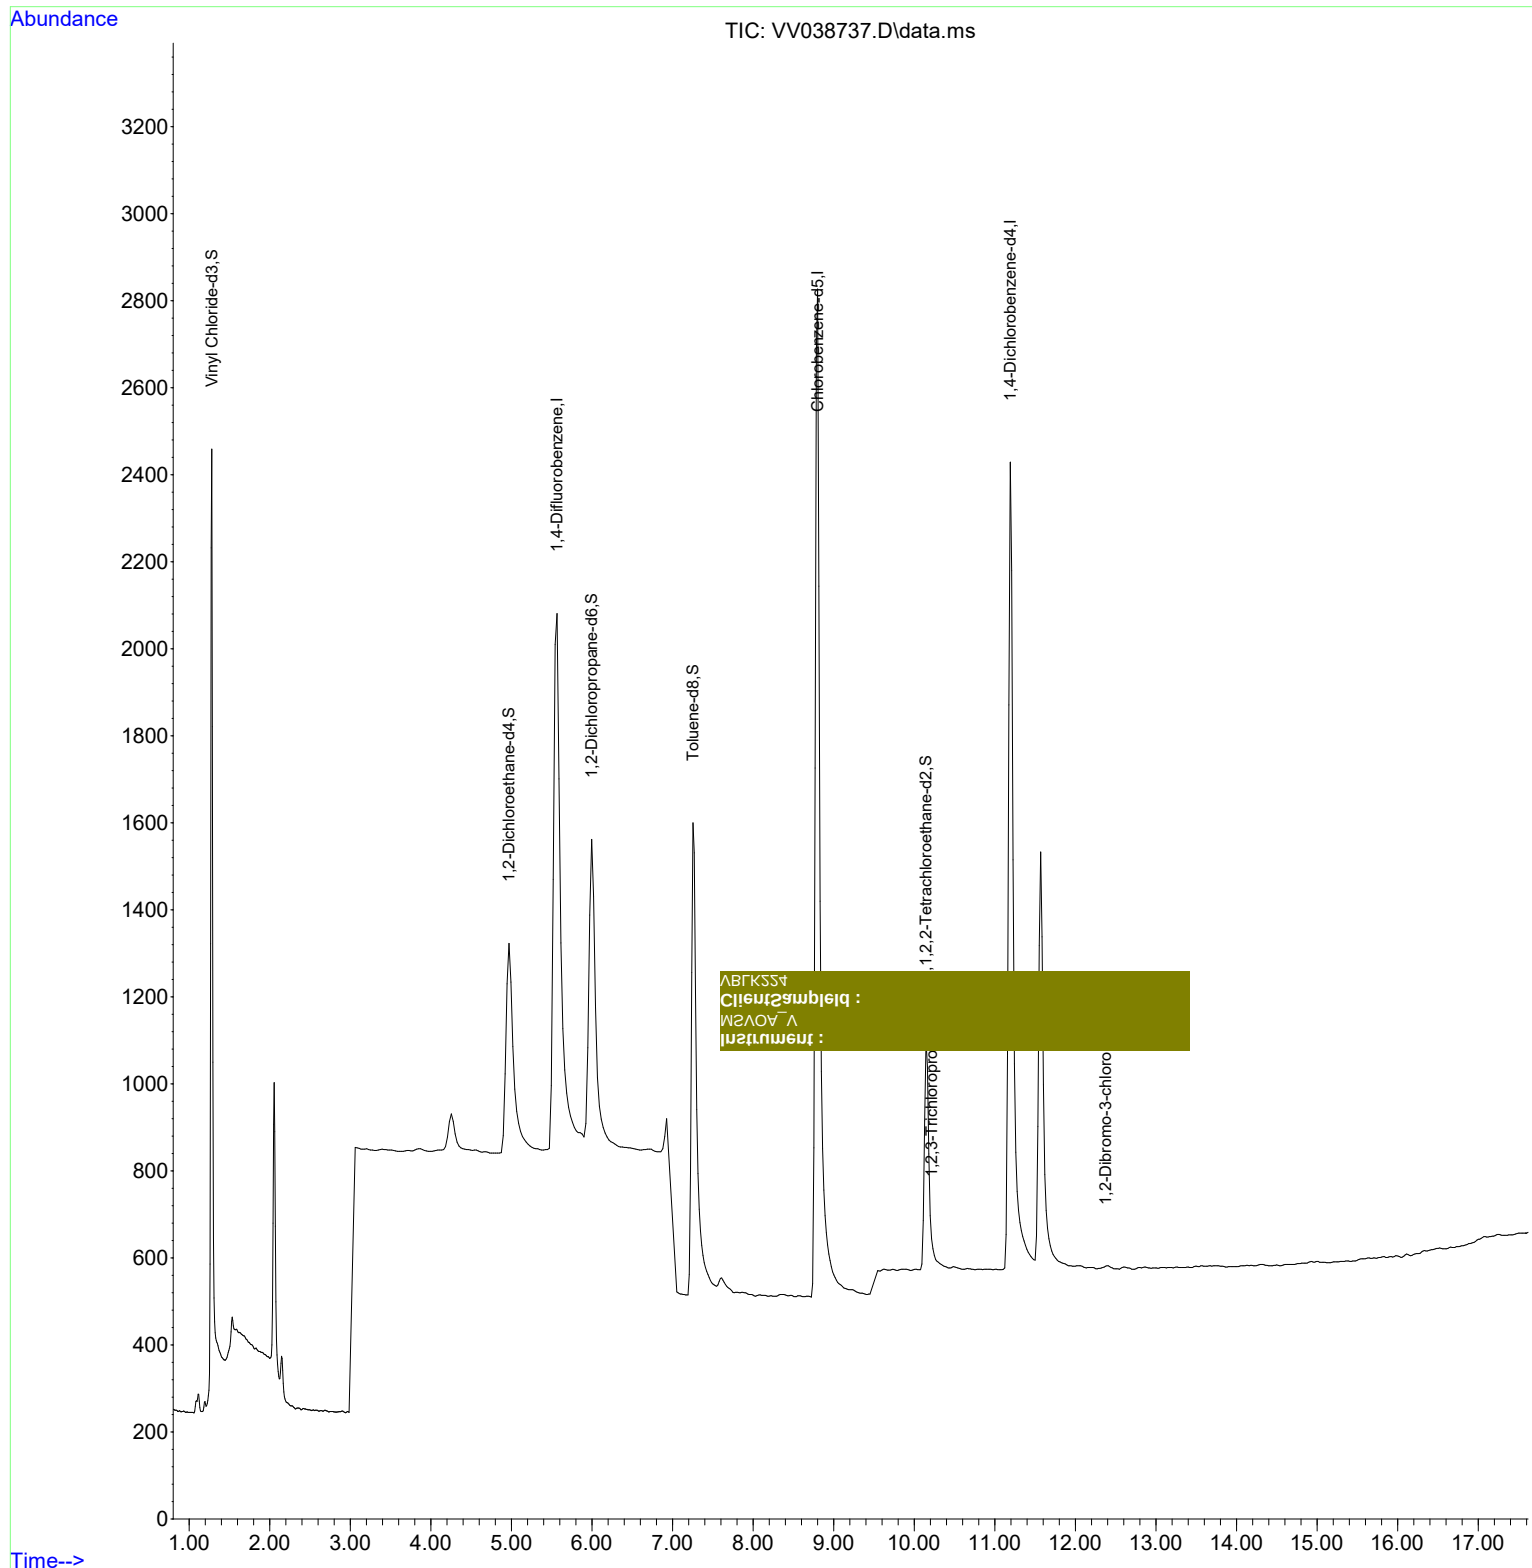

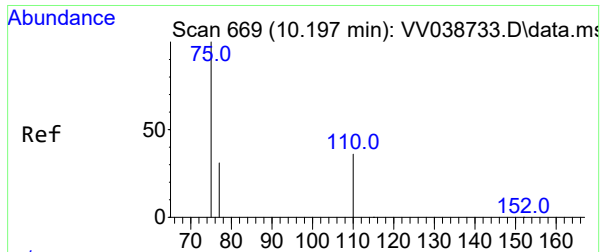




#12
1,2,3-Trichloropropane
Concen: 0.02 ug/L
RT: 10.214 min Scan# 670
Delta R.T. 0.017 min
Lab File: VV038737.D
Acq: 24 Mar 2025 14:05

Tgt Ion: 75 Resp: 45
Ion Ratio Lower Upper
75 100
110 31.1 33.4 50.0#
77 8.9 27.0 40.6#

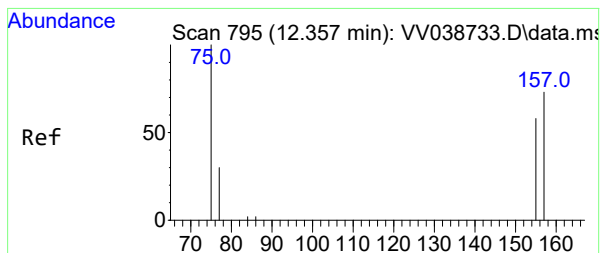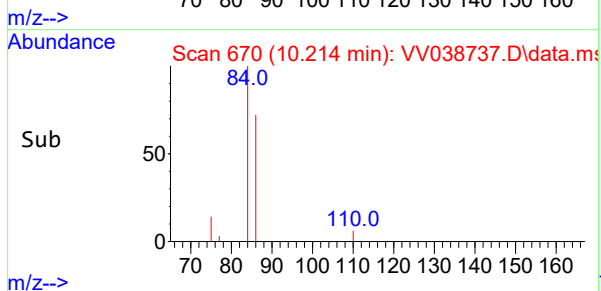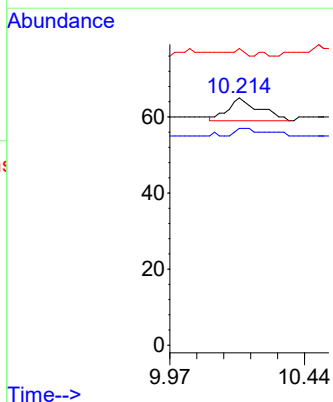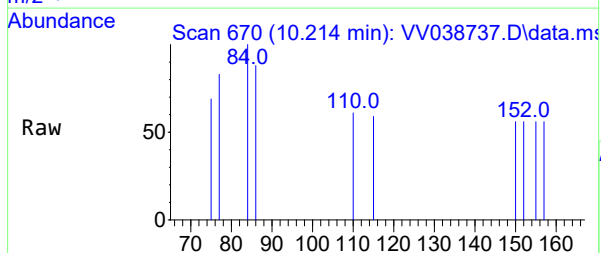

#13
1,2-Dibromo-3-chloropropane
Concen: 0.03 ug/L
RT: 12.374 min Scan# 796
Delta R.T. 0.017 min
Lab File: VV038737.D
Acq: 24 Mar 2025 14:05

Tgt Ion: 75 Resp: 17
Ion Ratio Lower Upper
75 100
157 85.7 81.1 121.7
155 85.7 70.3 105.5

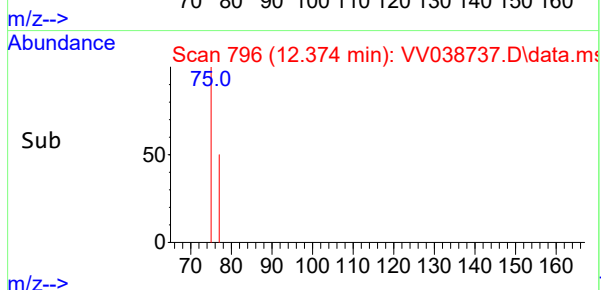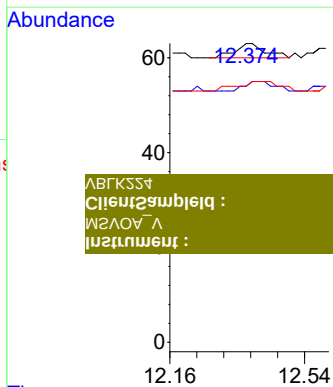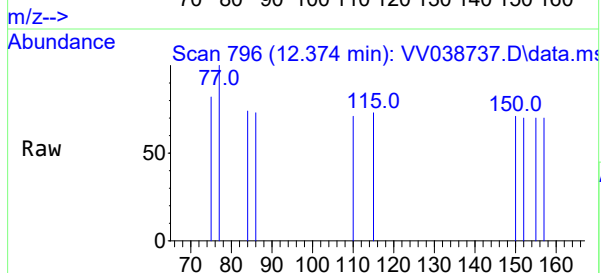

LABKSS
Client Sample ID :
MS/MS
Instrument :