

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032519\
 Data File : VV009862.D
 Acq On : 25 Mar 2019 15:44
 Operator : SY/MD
 Sample : VV0325WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032519WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.206	31	36	46	rBV2	11884	18829	2.32%	0.301%
2	1.322	66	72	83	rVB	168832	160991	19.87%	2.573%
3	1.563	142	147	160	rVB	154177	190109	23.46%	3.039%
4	2.126	314	322	335	rVB	397198	556161	68.64%	8.890%
5	2.463	421	427	429	rBV	1437	1300	0.16%	0.021%
6	2.582	461	464	468	rBV2	1191	808	0.10%	0.013%
7	2.605	469	471	474	rVB	1040	520	0.06%	0.008%
8	2.759	514	519	522	rBV3	1189	1150	0.14%	0.018%
9	2.830	538	541	543	rBV	1136	695	0.09%	0.011%
10	2.971	583	585	588	rBV3	1231	976	0.12%	0.016%
11	3.026	600	602	607	rVB3	1381	785	0.10%	0.013%
12	3.110	625	628	632	rBV3	681	430	0.05%	0.007%
13	3.370	707	709	710	rBV	942	411	0.05%	0.007%
14	3.470	737	740	742	rBV	1676	1021	0.13%	0.016%
15	3.560	765	768	770	rBV2	891	675	0.08%	0.011%
16	3.778	831	836	838	rBV2	1209	1039	0.13%	0.017%
17	3.794	838	841	844	rVB2	1218	856	0.11%	0.014%
18	3.881	865	868	870	rVB	1012	525	0.06%	0.008%
19	3.929	870	883	907	rBV	51046	134995	16.66%	2.158%
20	4.219	970	973	977	rBV	1203	1003	0.12%	0.016%
21	4.399	1012	1029	1053	rBV2	125185	314710	38.84%	5.031%
22	4.569	1079	1082	1084	rBV2	1595	1096	0.14%	0.018%
23	4.833	1161	1164	1166	rBV2	1099	622	0.08%	0.010%
24	4.904	1183	1186	1191	rBV4	1202	1466	0.18%	0.023%
25	5.023	1221	1223	1226	rVB2	1038	523	0.06%	0.008%
26	5.093	1226	1245	1268	rBV4	317144	810313	100.00%	12.953%
27	5.351	1321	1325	1326	rBV	1135	843	0.10%	0.013%
28	5.663	1408	1422	1443	rBV2	220711	444564	54.86%	7.106%
29	5.855	1480	1482	1485	rVB2	1563	749	0.09%	0.012%
30	5.875	1485	1488	1489	rBV	1078	594	0.07%	0.009%
31	5.900	1493	1496	1500	rVB4	1058	964	0.12%	0.015%
32	5.945	1503	1510	1511	rBV4	2908	2885	0.36%	0.046%
33	6.061	1543	1546	1547	rBV	1151	649	0.08%	0.010%
34	6.116	1550	1563	1582	rVV2	177778	365836	45.15%	5.848%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032519\
 Data File : VV009862.D
 Acq On : 25 Mar 2019 15:44
 Operator : SY/MD
 Sample : VV0325WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032519WMA.M
 Title : VOC Analysis

35	6.444	1662	1665	1670	rBV3	1121	957	0.12%	0.015%
36	6.470	1670	1673	1675	rBV2	1544	921	0.11%	0.015%
37	6.527	1685	1691	1698	rVB2	1431	1874	0.23%	0.030%
38	6.560	1698	1701	1705	rBV2	1078	902	0.11%	0.014%
39	6.733	1751	1755	1756	rBV2	1223	876	0.11%	0.014%
40	6.855	1791	1793	1796	rBV	1090	511	0.06%	0.008%
41	6.945	1818	1821	1824	rBV3	902	709	0.09%	0.011%
42	7.026	1833	1846	1859	rBV2	87837	162219	20.02%	2.593%
43	7.283	1923	1926	1928	rBV2	919	439	0.05%	0.007%
44	7.357	1937	1949	1968	rBV	357442	638292	78.77%	10.203%
45	7.662	2033	2044	2059	rBV	64107	106680	13.17%	1.705%
46	7.791	2081	2084	2087	rBV2	1364	1057	0.13%	0.017%
47	7.865	2104	2107	2108	rBV	690	431	0.05%	0.007%
48	7.974	2136	2141	2144	rBV3	1787	1518	0.19%	0.024%
49	8.132	2178	2190	2206	rBV	165990	297714	36.74%	4.759%
50	8.338	2252	2254	2256	rBV2	1080	603	0.07%	0.010%
51	8.457	2289	2291	2296	rBV	1292	1224	0.15%	0.020%
52	8.486	2298	2300	2306	rVB2	1715	1154	0.14%	0.018%
53	8.592	2330	2333	2335	rBV2	1158	688	0.08%	0.011%
54	8.624	2340	2343	2345	rBV2	840	584	0.07%	0.009%
55	8.723	2371	2374	2377	rBV	1172	861	0.11%	0.014%
56	8.826	2403	2406	2408	rBV2	1324	1078	0.13%	0.017%
57	8.894	2416	2427	2443	rBV	347231	568731	70.19%	9.091%
58	9.132	2498	2501	2503	rBV	976	652	0.08%	0.010%
59	9.325	2557	2561	2563	rBV2	1032	861	0.11%	0.014%
60	9.434	2591	2595	2598	rBV	1411	1441	0.18%	0.023%
61	9.486	2608	2611	2616	rBV3	1316	1258	0.16%	0.020%
62	9.887	2731	2736	2738	rBV	1155	887	0.11%	0.014%
63	9.965	2756	2760	2764	rBV2	1199	1440	0.18%	0.023%
64	10.022	2775	2778	2784	rVB	2026	1688	0.21%	0.027%
65	10.051	2784	2787	2791	rBV	1213	1056	0.13%	0.017%
66	10.132	2810	2812	2814	rBV	716	443	0.05%	0.007%
67	10.260	2842	2852	2872	rVB	236346	372737	46.00%	5.958%
68	10.399	2892	2895	2896	rBV3	930	605	0.07%	0.010%
69	10.540	2936	2939	2948	rVB3	1647	2328	0.29%	0.037%
70	10.646	2969	2972	2975	rBV	843	681	0.08%	0.011%
71	10.678	2980	2982	2985	rBV2	886	504	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032519\
 Data File : VV009862.D
 Acq On : 25 Mar 2019 15:44
 Operator : SY/MD
 Sample : VV0325WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032519WMA.M
 Title : VOC Analysis

72	10.765	3007	3009	3015	rBV3	786	708	0.09%	0.011%
73	10.791	3015	3017	3022	rBV	694	741	0.09%	0.012%
74	10.887	3044	3047	3049	rBV2	696	470	0.06%	0.008%
75	10.971	3071	3073	3076	rBV3	1023	561	0.07%	0.009%
76	11.235	3147	3155	3162	rBV5	2499	3777	0.47%	0.060%
77	11.296	3162	3174	3192	rBV	296756	486812	60.08%	7.782%
78	11.559	3253	3256	3260	rBV	1273	869	0.11%	0.014%
79	11.672	3280	3291	3307	rBV	335651	546393	67.43%	8.734%
80	11.955	3375	3379	3382	rBV	1034	999	0.12%	0.016%
81	12.913	3672	3677	3679	rBV	1220	1078	0.13%	0.017%
82	13.083	3725	3730	3732	rBV	1301	1145	0.14%	0.018%
83	13.190	3759	3763	3765	rBV	1025	922	0.11%	0.015%
84	13.251	3779	3782	3787	rBV2	941	775	0.10%	0.012%
85	13.389	3823	3825	3829	rBV	881	646	0.08%	0.010%
86	13.434	3836	3839	3841	rBV4	1073	710	0.09%	0.011%
87	13.614	3892	3895	3902	rVB2	1414	1125	0.14%	0.018%
88	13.649	3903	3906	3913	rVV	779	685	0.08%	0.011%
89	13.932	3990	3994	3998	rBV2	1256	1479	0.18%	0.024%
90	14.077	4036	4039	4047	rBV3	1874	1821	0.22%	0.029%
91	14.222	4081	4084	4086	rBV2	818	479	0.06%	0.008%
92	14.280	4099	4102	4103	rBV2	1254	789	0.10%	0.013%
93	14.771	4252	4255	4257	rBV	1232	828	0.10%	0.013%
94	14.890	4289	4292	4294	rBV2	1596	796	0.10%	0.013%
95	14.932	4302	4305	4307	rBV	1305	1046	0.13%	0.017%
96	14.987	4319	4322	4324	rBV2	953	630	0.08%	0.010%
97	15.119	4360	4363	4364	rBV2	891	587	0.07%	0.009%
98	15.447	4461	4465	4469	rBV	1971	1656	0.20%	0.026%
99	15.865	4593	4595	4600	rBV4	1092	987	0.12%	0.016%
100	16.045	4648	4651	4652	rBV	1039	553	0.07%	0.009%


Sum of corrected areas: 6255764

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032519\
Data File : VV009862.D
Acq On : 25 Mar 2019 15:44
Operator : SY/MD
Sample : VV0325WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK78

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

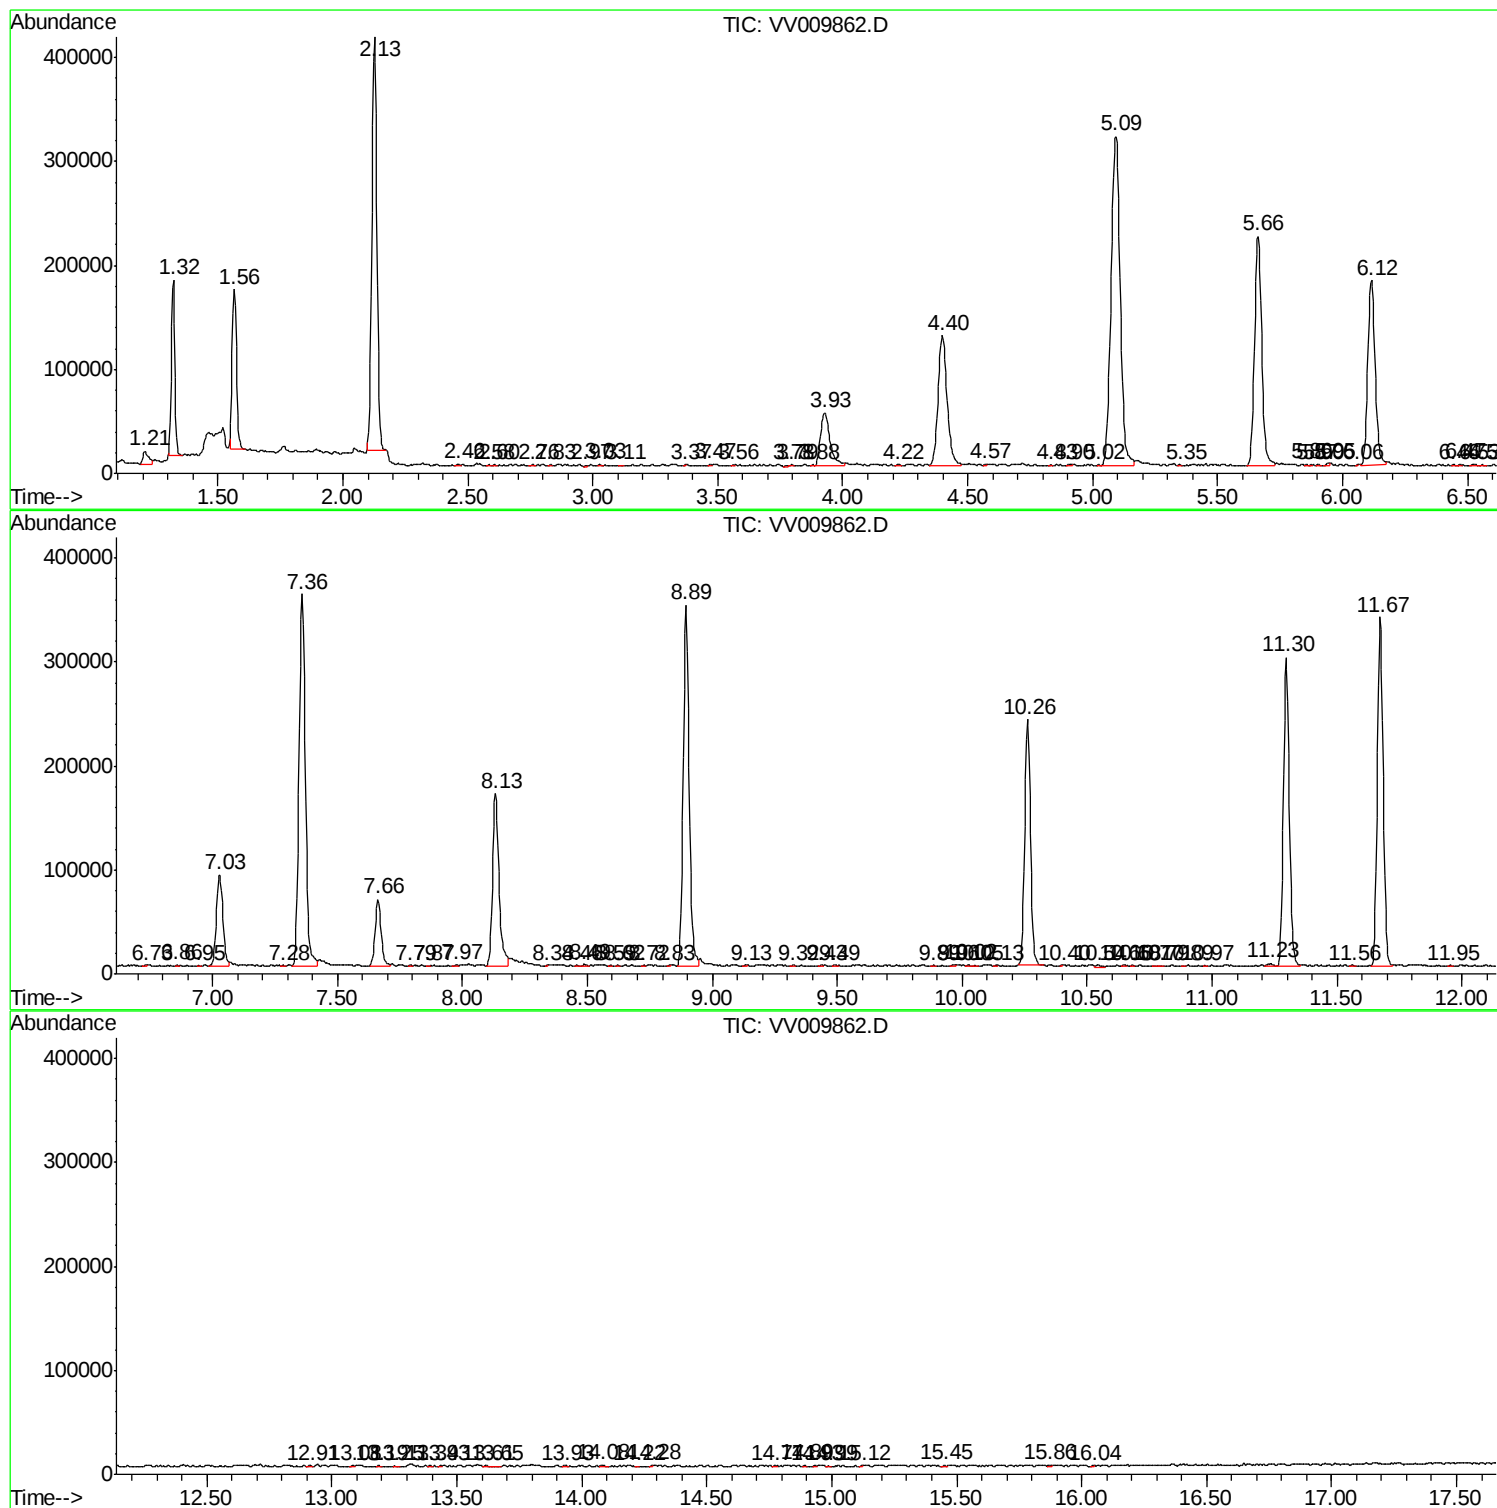

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032519\
Data File : VV009862.D
Acq On : 25 Mar 2019 15:44
Operator : SY/MD
Sample : VV0325WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK78

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032519\
Data File : VV009862.D
Acq On : 25 Mar 2019 15:44
Operator : SY/MD
Sample : VV0325WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK78

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc