


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV032519\
 Data File : VV009851.D
 Acq On : 25 Mar 2019 09:09
 Operator : SY/MD
 Sample : BFB82
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB82

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032519WMA.M
 Title : VOC Analysis
 Last Update : Tue Mar 26 07:13:38 2019

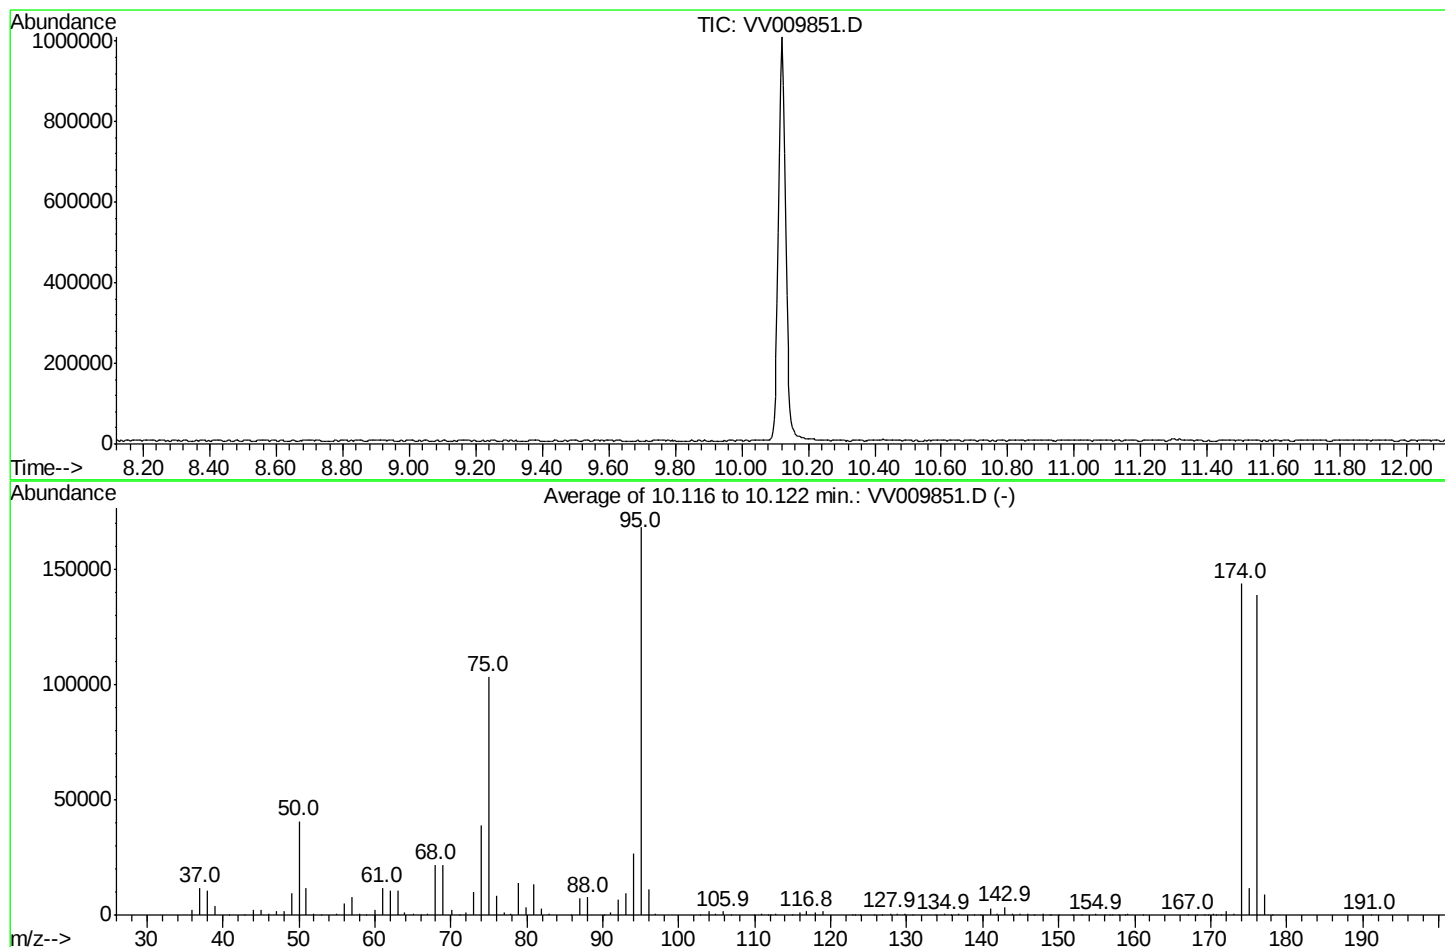

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	40728	PASS
75	95	30	80	61.4	103392	PASS
95	95	100	100	100.0	168341	PASS
96	95	5	9	6.6	11091	PASS
173	174	0.00	2	0.5	721	PASS
174	95	50	120	85.4	143816	PASS
175	174	5	9	8.0	11532	PASS
176	174	95	101	96.8	139232	PASS
177	176	5	9	6.3	8726	PASS

Scan 2794 (10.074 min): VV009851.D
BFB82

m/z	Abundance
36.00	110.0
38.80	128.0
39.90	8007.0
43.80	102.0
44.20	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	2153.0
37.00	11376.0
38.00	10199.0
39.00	3934.0
40.00	8054.0
40.90	193.0
44.00	2275.0
45.00	1835.0
46.00	355.0
47.00	1920.0
48.00	1682.0
49.00	8552.0
50.00	39616.0
51.00	10623.0
52.00	530.0
52.90	100.0
55.00	633.0
55.90	4590.0
57.00	7483.0
58.00	334.0
58.90	118.0
59.90	2076.0
61.00	11381.0
62.00	10590.0
63.00	10080.0
64.00	1024.0
65.00	849.0
66.10	111.0
67.00	684.0
68.00	20072.0
69.00	20424.0
70.10	2000.0
72.00	1206.0
73.00	9482.0
74.00	37144.0
75.00	98448.0
76.00	7965.0
77.10	1331.0
78.00	457.0
78.90	13233.0
80.00	3267.0
80.90	12604.0
81.90	2908.0
82.90	466.0
85.90	156.0
87.00	6740.0
88.00	7503.0
90.20	224.0
91.00	1437.0
92.00	6247.0
93.00	8939.0
94.00	25760.0
95.00	156608.0
96.00	10567.0
96.90	393.0
102.90	132.0
104.00	1333.0
104.90	329.0
105.90	1440.0
106.80	292.0
109.90	278.0
110.90	270.0
111.80	192.0
112.80	353.0
114.90	134.0
115.90	831.0
116.80	1579.0
117.90	1111.0
118.90	1299.0
122.80	109.0
123.20	140.0
123.80	309.0
127.90	713.0
128.80	403.0
129.80	638.0
130.90	236.0
134.90	572.0
136.80	448.0
141.00	2615.0
141.90	471.0
142.90	3211.0
143.90	276.0
144.90	455.0
145.90	344.0
147.90	445.0
148.70	128.0
150.00	281.0
151.90	144.0
152.90	125.0
154.90	370.0
156.80	181.0
157.10	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

157.90	122.0
158.70	222.0
159.10	345.0
167.00	122.0
168.10	117.0
169.20	156.0
169.70	104.0
170.50	308.0
171.30	552.0
172.00	1342.0
173.00	2163.0
174.00	130392.0
175.00	10529.0
176.00	123616.0
177.00	8288.0
178.20	261.0
191.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	2427.0
37.00	12409.0
38.00	11052.0
39.00	4401.0
40.00	7933.0
40.90	169.0
42.80	137.0
44.00	2456.0
45.00	2084.0
46.00	395.0
47.00	1992.0
48.00	1903.0
49.00	9715.0
50.00	42288.0
51.00	11891.0
51.90	604.0
52.90	119.0
55.00	630.0
56.00	5053.0
57.00	7872.0
58.00	343.0
60.00	2458.0
61.00	12261.0
62.00	10929.0
63.00	10977.0
64.00	1325.0
65.00	836.0
67.00	860.0
68.00	22616.0
69.00	22392.0
70.10	2173.0
72.00	1220.0
73.00	10324.0
74.00	40776.0
75.00	107584.0
76.00	8440.0
77.10	1327.0
77.90	565.0
78.90	14309.0
79.90	3571.0
80.90	13979.0
81.90	3015.0
82.90	500.0
85.80	201.0
87.00	7644.0
88.00	7942.0
91.00	1436.0
92.00	7038.0
93.00	9837.0
94.00	27664.0
95.00	174976.0
96.00	11515.0
96.90	376.0
102.90	178.0
103.90	1441.0
104.90	450.0
105.90	1510.0
106.80	284.0
109.90	299.0
110.90	323.0
111.80	225.0
112.80	456.0
114.90	254.0
115.90	934.0
116.80	1669.0
117.90	1167.0
118.90	1511.0
123.20	138.0
123.80	315.0
125.70	123.0
126.70	141.0
127.90	787.0
128.80	400.0
129.80	689.0
130.80	233.0
135.00	560.0
135.80	110.0
136.90	594.0
138.90	126.0
141.00	3060.0
142.00	515.0
142.90	3562.0
144.00	321.0
145.00	391.0
145.90	333.0
147.90	533.0
149.00	165.0
150.00	230.0
151.80	142.0
152.90	143.0
154.90	405.0
156.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

156.70	247.0
157.90	138.0
159.10	364.0
167.00	139.0
168.20	159.0
169.20	190.0
169.70	159.0
170.30	347.0
172.00	1527.0
174.00	149120.0
175.00	12090.0
176.00	144640.0
177.00	9110.0
178.10	316.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	2420.0
37.00	11974.0
38.00	10490.0
39.00	4519.0
40.00	7827.0
40.90	122.0
42.80	178.0
44.00	2321.0
45.00	2020.0
46.10	408.0
47.00	1810.0
48.00	1880.0
49.00	9535.0
50.00	40280.0
51.00	12030.0
51.90	619.0
52.90	117.0
55.00	627.0
56.00	5042.0
57.00	7411.0
58.00	387.0
60.00	2364.0
61.00	11417.0
62.00	10960.0
63.00	10425.0
63.90	1398.0
65.00	820.0
67.00	829.0
68.00	22408.0
69.00	21896.0
70.10	1974.0
71.20	184.0
72.00	1309.0
73.00	10430.0
74.00	39488.0
75.00	104144.0
76.00	8274.0
77.10	1230.0
77.80	617.0
78.90	13968.0
79.90	3594.0
80.90	13980.0
81.90	2849.0
82.90	528.0
85.80	214.0
87.00	7677.0
88.00	7397.0
90.90	1159.0
92.00	6826.0
93.00	9754.0
94.00	26072.0
95.00	173440.0
96.00	11191.0
97.00	320.0
102.80	267.0
103.90	1468.0
104.80	496.0
105.90	1432.0
106.80	227.0
109.90	258.0
110.90	338.0
112.10	243.0
112.80	465.0
114.90	364.0
115.90	978.0
116.80	1529.0
117.90	1034.0
118.90	1517.0
123.80	224.0
125.70	120.0
126.80	140.0
127.90	735.0
128.80	318.0
129.80	724.0
130.70	274.0
133.80	108.0
135.00	490.0
135.90	105.0
136.90	659.0
138.90	123.0
139.70	112.0
141.00	3245.0
141.90	456.0
142.90	3550.0
144.00	323.0
144.90	351.0
145.90	335.0
146.70	101.0
147.90	583.0
149.00	147.0
150.00	225.0
151.80	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

153.00	111.0
154.90	346.0
155.90	105.0
156.70	308.0
157.90	115.0
159.00	300.0
161.10	126.0
168.20	207.0
169.20	151.0
170.30	340.0
170.60	372.0
172.00	1528.0
174.00	151936.0
175.00	11977.0
176.00	149440.0
177.00	8780.0
178.00	300.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82