

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV032525\
Data File : VV038742.D
Acq On : 25 Mar 2025 09:29
Operator : SY/MD
Sample : VV0325WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 25 09:48:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM032425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Mar 24 15:12:15 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5512	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5202	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2254	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2561	0.50	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 100.00%			
4) 1,2-Dichloroethane-d4	4.969	65	1333	0.51	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 102.00%			
7) 1,2-Dichloropropane-d6	5.995	67	1568	0.49	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 98.00%			
8) Toluene-d8	7.253	98	3036	0.51	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 102.00%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	1287	0.47	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 94.00%			
Target Compounds						
12) 1,2,3-Trichloropropane	10.060	75	56	0.02	ug/L	Qvalue # 40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

LABKSSP
Client Sample ID :
MSVOA_V
Instrument :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV032525\
Data File : VV038742.D
Acq On : 25 Mar 2025 09:29
Operator : SY/MD
Sample : VV0325WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1




Quant Time: Mar 25 09:48:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM032425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Mar 24 15:12:15 2025
Response via : Initial Calibration

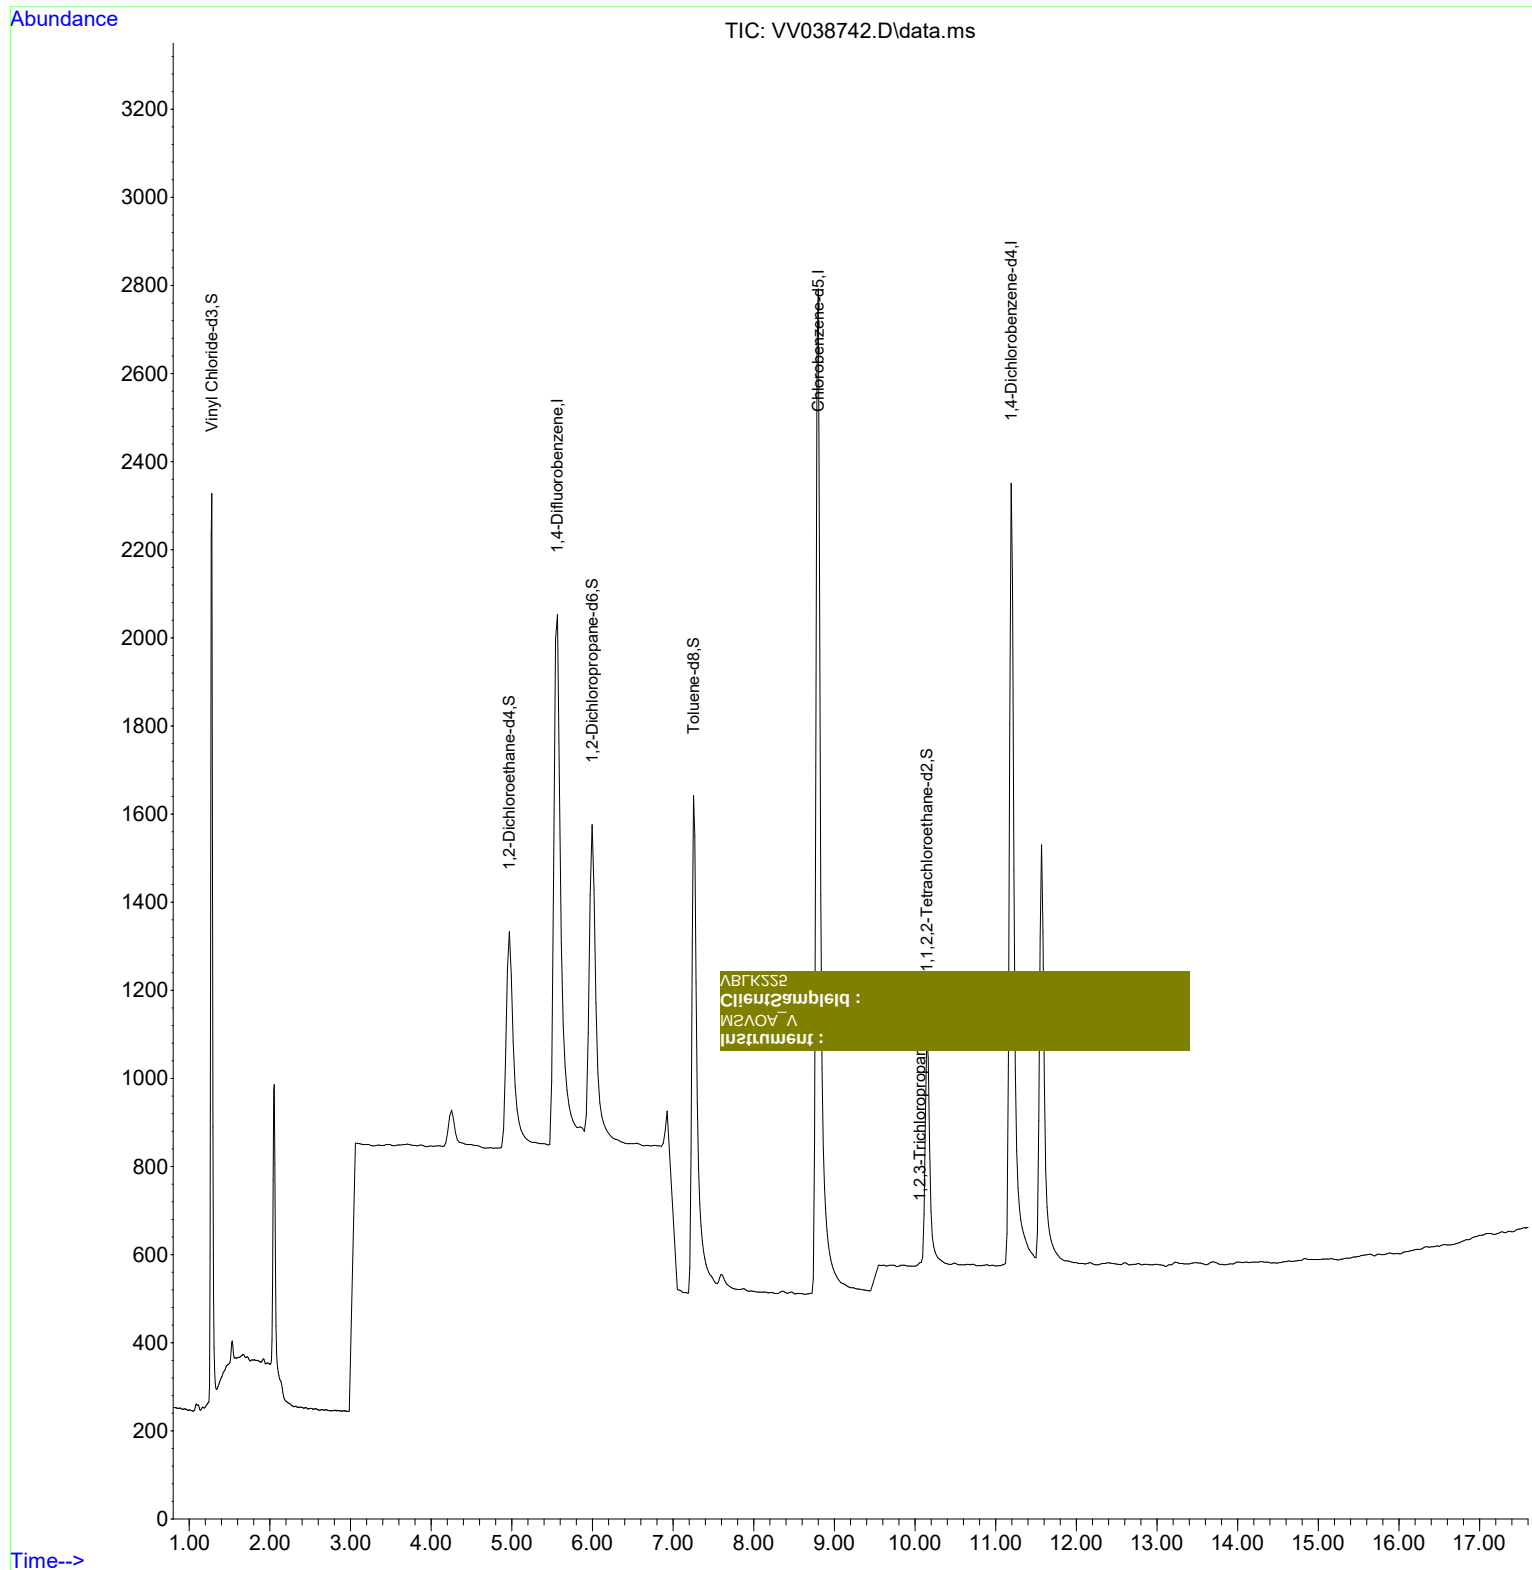

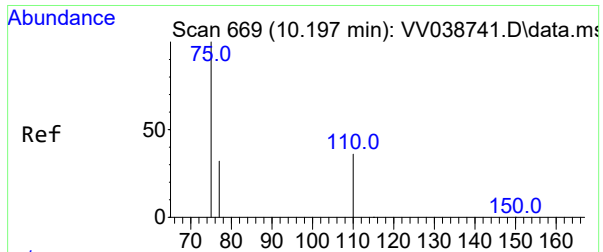

#12
 1,2,3-Trichloropropane
 Concen: 0.02 ug/L
 RT: 10.060 min Scan# 661
 Delta R.T. -0.137 min
 Lab File: VV038742.D
 Acq: 25 Mar 2025 09:29

Tgt Ion: 75 Resp: 56
 Ion Ratio Lower Upper
 75 100
 110 0.0 33.4 50.0#
 77 3.6 27.0 40.6#

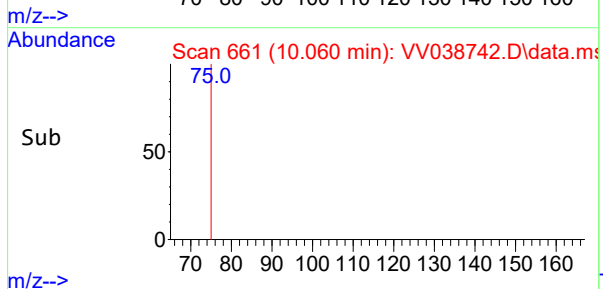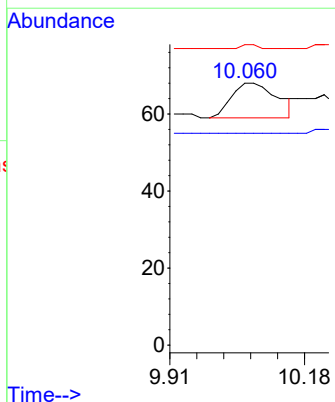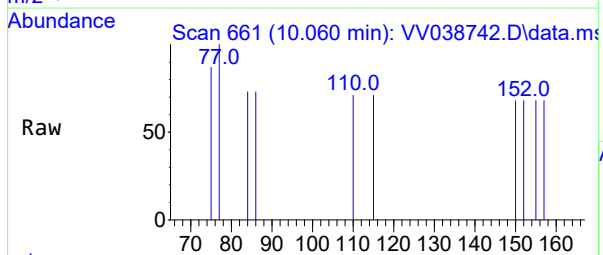

LABKSSP
 Client Sample ID :
 MS/MS
 Instrument :