

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV032525\
 Data File : VV038743.D
 Acq On : 25 Mar 2025 10:47
 Operator : SY/MD
 Sample : Q1546-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Mar 25 11:42:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM032425.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Mar 24 15:12:15 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5180	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	4936	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2168	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2317	0.48	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	96.00%		
4) 1,2-Dichloroethane-d4	4.969	65	1170	0.47	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.00%		
7) 1,2-Dichloropropane-d6	5.995	67	1417	0.46	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	92.00%		
8) Toluene-d8	7.253	98	2702	0.47	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.00%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	1179	0.46	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	92.00%		
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	255	0.03	ug/L #	1
6) Trichloroethene	5.876	95	109	0.02	ug/L #	89
12) 1,2,3-Trichloropropane	10.214	75	67	0.03	ug/L #	57
13) 1,2-Dibromo-3-chloropr...	12.374	75	17	0.03	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

MDT-WATER-01T-S032-05
 Client Sample ID :
 MSVOA_V
 Instrument :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV032525\
Data File : VV038743.D
Acq On : 25 Mar 2025 10:47
Operator : SY/MD
Sample : Q1546-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1





Quant Time: Mar 25 11:42:40 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM032425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Mar 24 15:12:15 2025
Response via : Initial Calibration

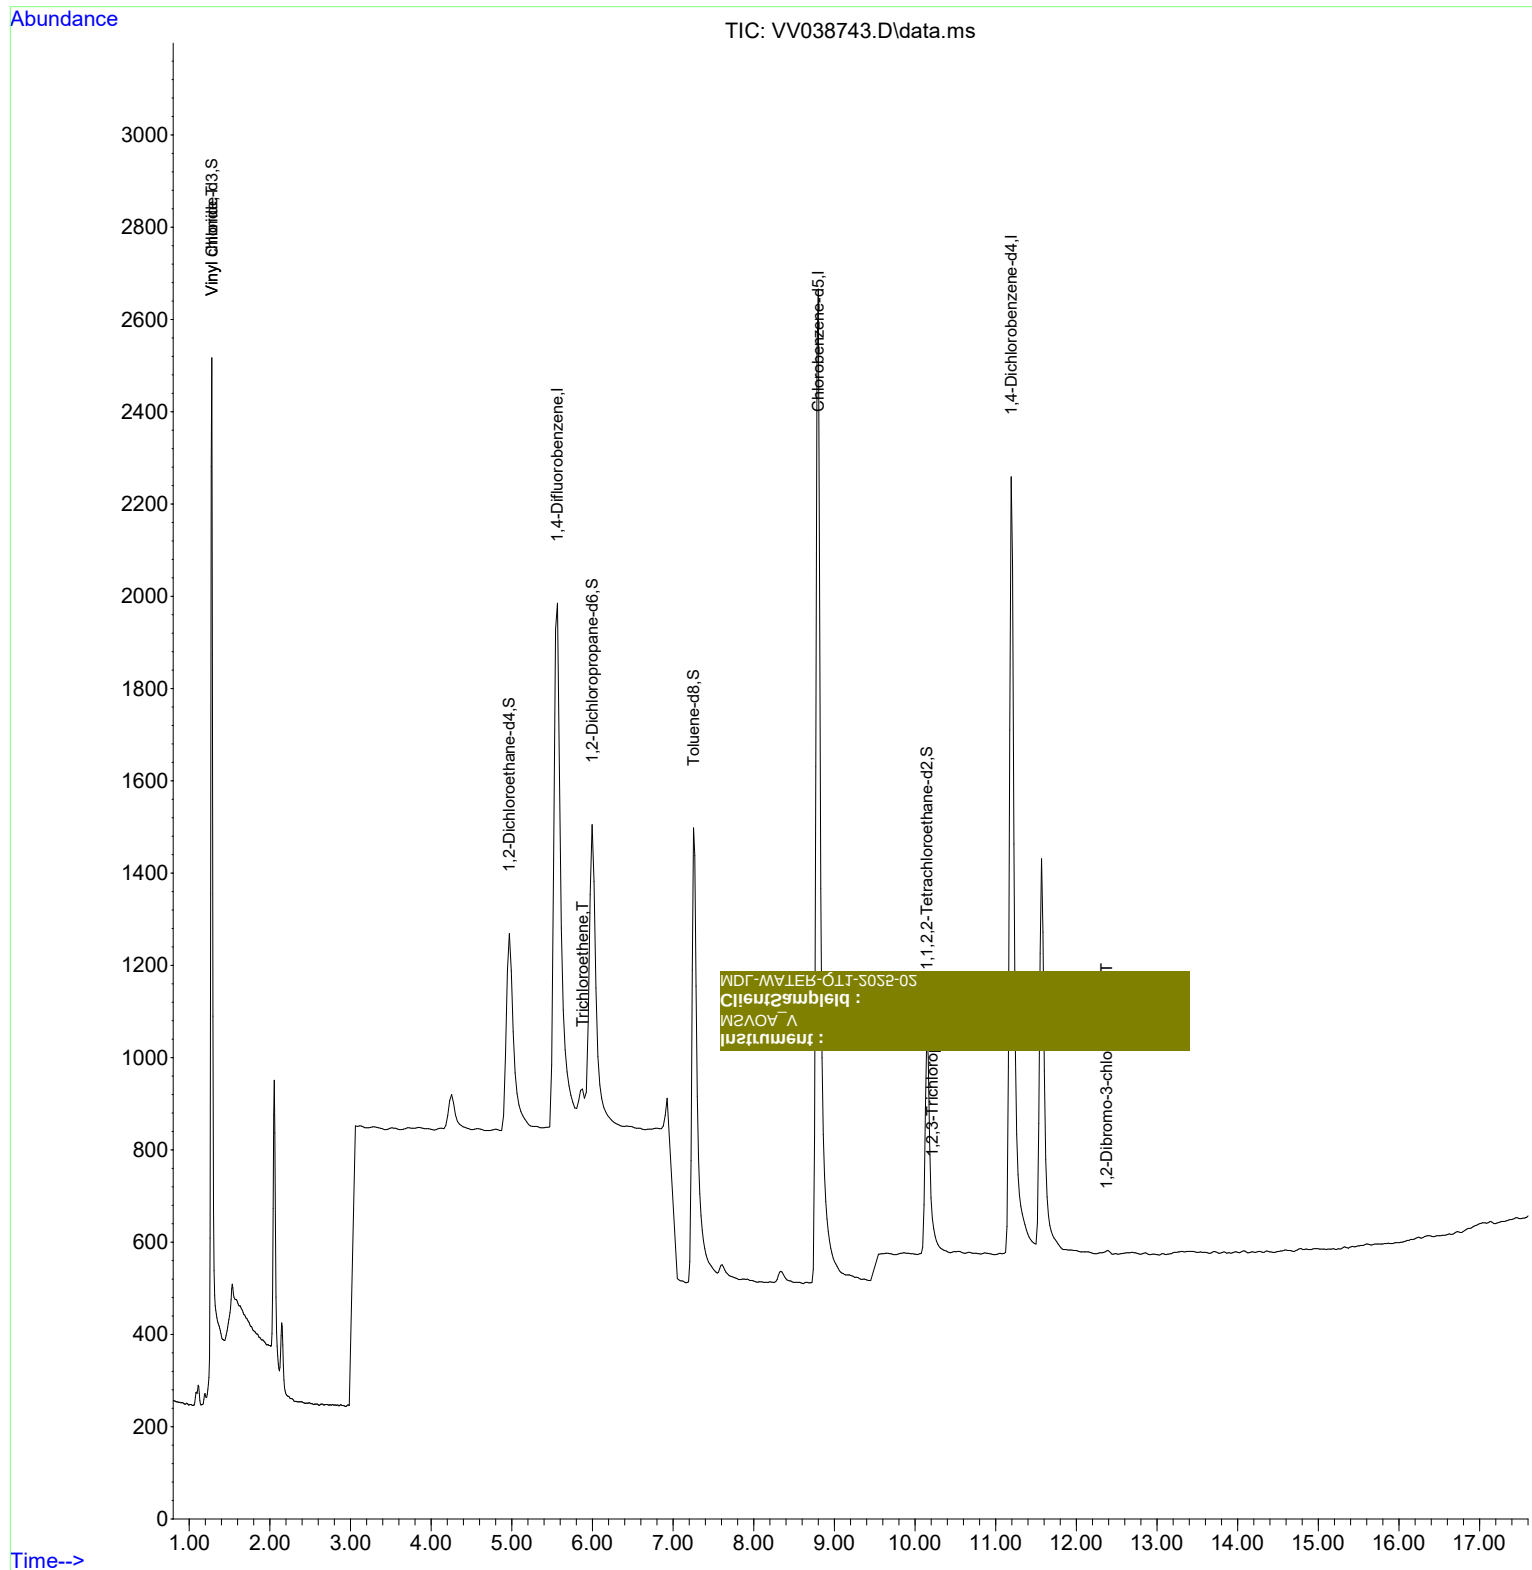

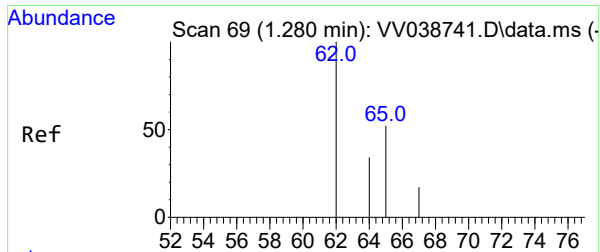




#3
 Vinyl chloride
 Concen: 0.03 ug/L
 RT: 1.280 min Scan# 69
 Delta R.T. -0.000 min
 Lab File: VV038743.D
 Acq: 25 Mar 2025 10:47

Tgt Ion: 62 Resp: 255
 Ion Ratio Lower Upper
 62 100
 64 132.1 23.4 43.4#

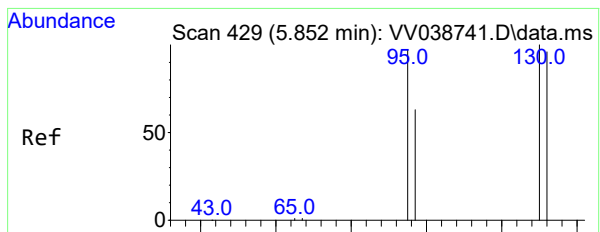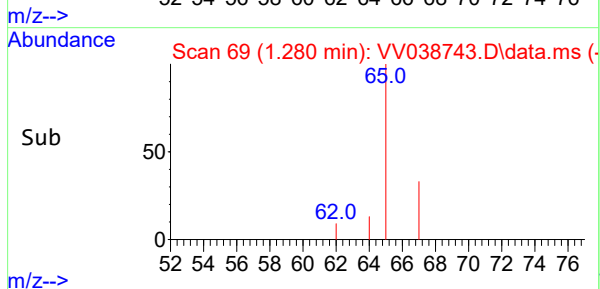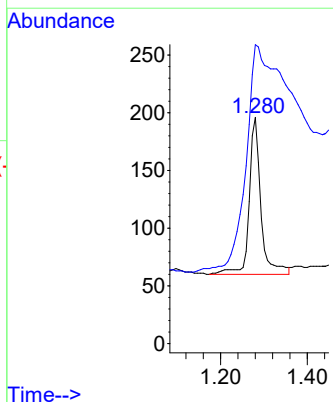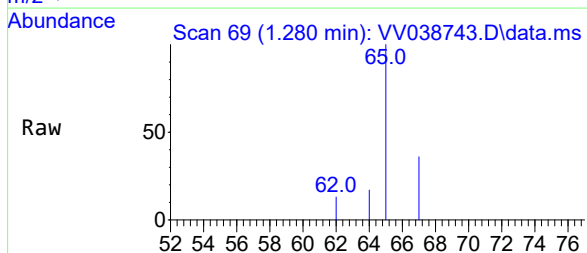


#6
 Trichloroethene
 Concen: 0.02 ug/L
 RT: 5.876 min Scan# 430
 Delta R.T. 0.024 min
 Lab File: VV038743.D
 Acq: 25 Mar 2025 10:47

Tgt Ion: 95 Resp: 109
 Ion Ratio Lower Upper
 95 100
 97 90.7 46.5 86.5#
 132 96.0 68.4 127.0
 130 96.0 71.6 133.0


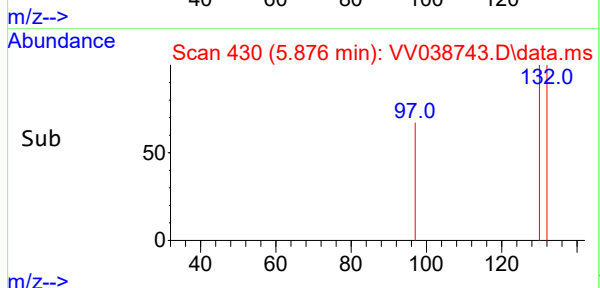
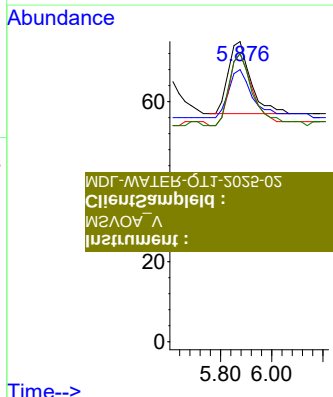
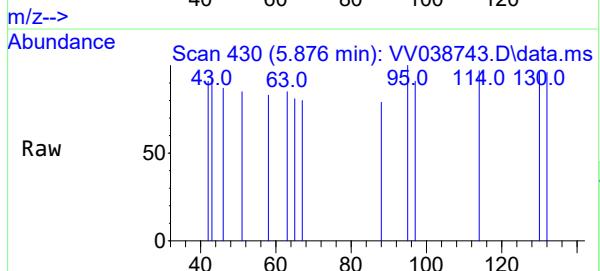


MDT-MATEB-01T-S032-05
 Client Sample ID :
 MS/MS
 Instrument :

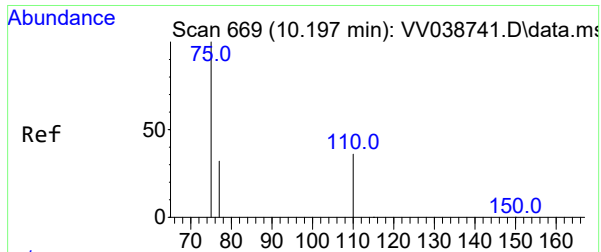




#12
1,2,3-Trichloropropane
Concen: 0.03 ug/L
RT: 10.214 min Scan# 670
Delta R.T. 0.017 min
Lab File: VV038743.D
Acq: 25 Mar 2025 10:47

Tgt Ion: 75 Resp: 67
Ion Ratio Lower Upper
75 100
110 80.6 33.4 50.0#
77 44.8 27.0 40.6#

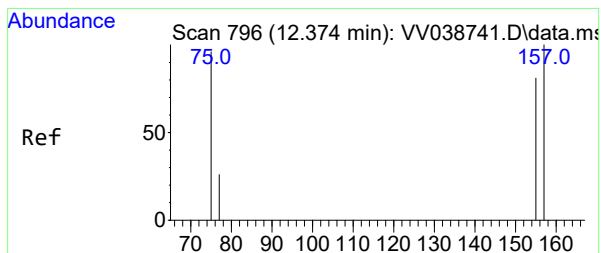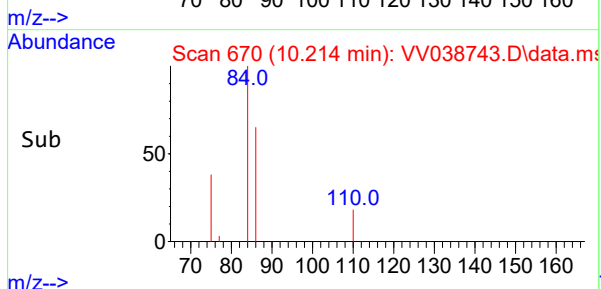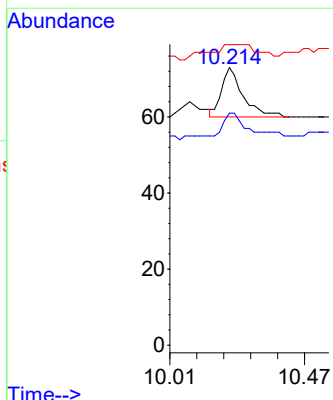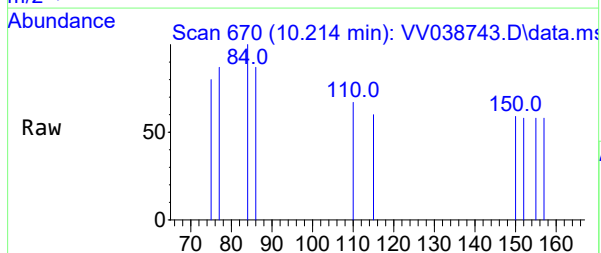

#13
1,2-Dibromo-3-chloropropane
Concen: 0.03 ug/L
RT: 12.374 min Scan# 796
Delta R.T. 0.017 min
Lab File: VV038743.D
Acq: 25 Mar 2025 10:47

Tgt Ion: 75 Resp: 17
Ion Ratio Lower Upper
75 100
157 87.3 81.1 121.7
155 85.7 70.3 105.5

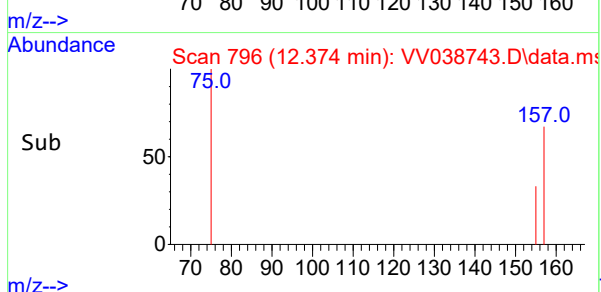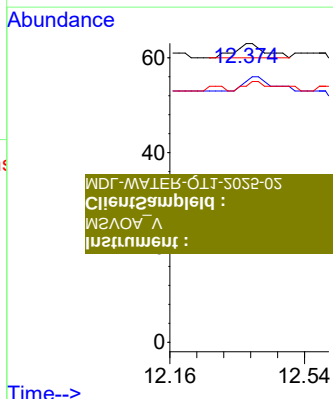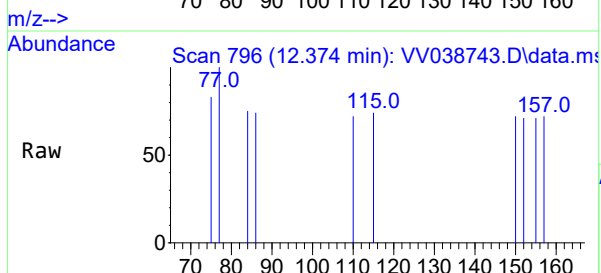

MDT-MATEB-01T-S0S2-05
Client Sample ID :
MS/MS
Instrument :