
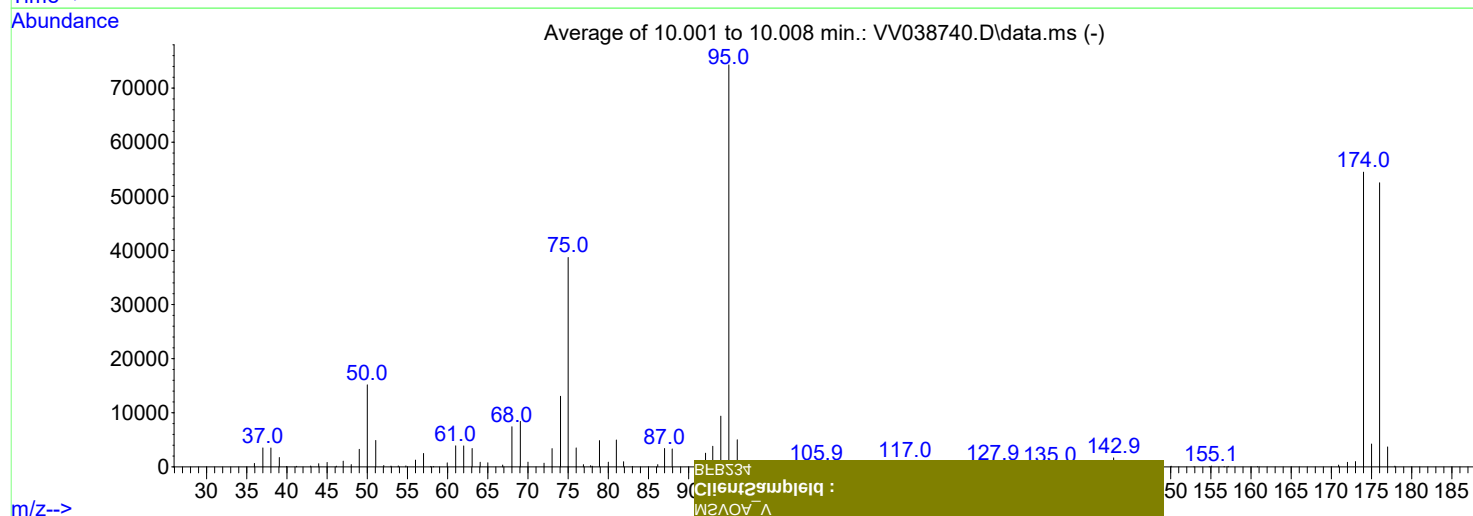


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV032525\
Data File : VV038740.D
Acq On : 25 Mar 2025 08:29
Operator : SY/MD
Sample : BFB234
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM032425.M
Title : TRACE VOA SOM01.0
Last Update : Mon Mar 24 15:12:15 2025

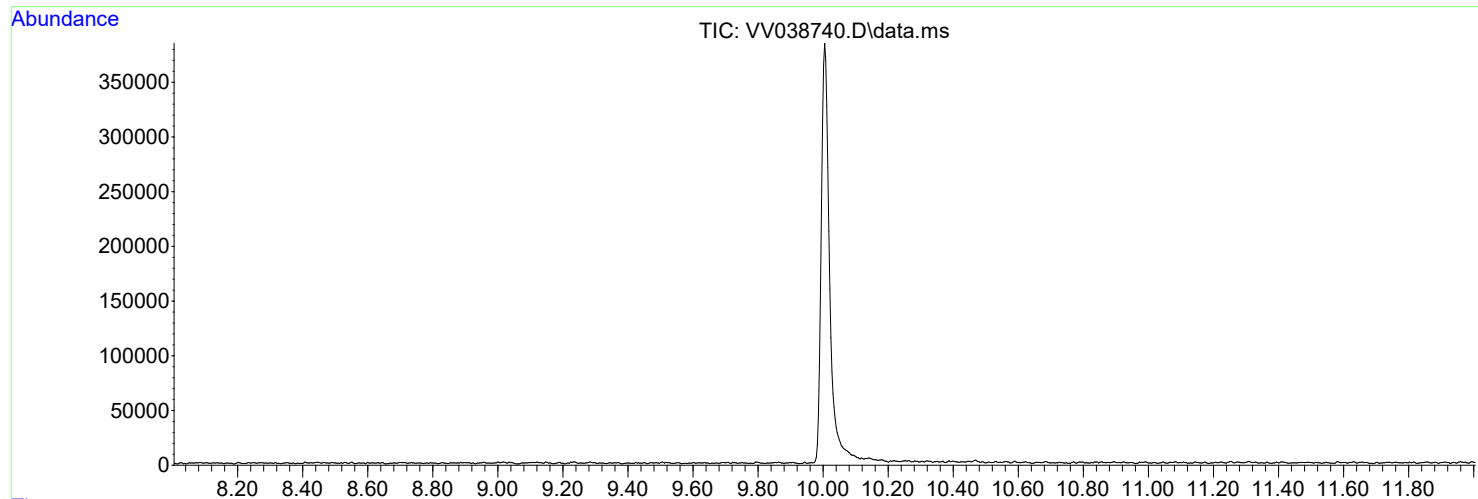

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2774

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	15162	PASS
75	95	30	80	52.1	38696	PASS
95	95	100	100	100.0	74291	PASS
96	95	5	9	6.8	5015	PASS
173	174	0.00	2	1.8	991	PASS
174	95	50	120	73.3	54475	PASS
175	174	5	9	7.8	4228	PASS
176	174	95	101	96.4	52509	PASS
177	176	5	9	7.0	3690	PASS

m/z	Abundance
35.10	132.0
35.80	131.0
36.50	104.0
40.00	326.0
40.90	185.0
41.80	125.0
44.00	496.0
45.60	102.0
46.00	119.0
54.80	104.0
77.00	127.0
80.10	114.0
107.70	113.0

BFB234
Client Sample :
MS/MS
Instrument :

m/z	Abundance
36.00	902.0
37.00	3699.0
38.00	3423.0
39.00	1731.0
39.90	421.0
40.70	189.0
42.00	104.0
43.00	157.0
44.00	1022.0
45.00	837.0
46.20	215.0
47.10	1148.0
48.00	470.0
49.00	3204.0
50.00	15333.0
51.00	4721.0
52.00	246.0
53.00	129.0
53.90	151.0
54.80	249.0
56.00	1117.0
57.00	2297.0
58.30	102.0
59.90	739.0
61.00	3657.0
62.00	3892.0
63.00	3509.0
64.10	833.0
65.00	634.0
66.80	267.0
68.00	7252.0
69.00	8268.0
70.00	857.0
72.00	694.0
73.00	3373.0
74.00	13172.0
75.00	38328.0
76.00	3342.0
76.90	587.0
77.80	309.0
78.90	4729.0
80.00	991.0
81.00	4887.0
81.90	863.0
86.10	383.0
87.00	3449.0
88.00	3418.0
90.80	378.0
92.10	2657.0
93.00	3664.0
94.00	8892.0
95.00	74128.0
96.00	4897.0
96.90	265.0
102.70	156.0
104.10	423.0
105.00	107.0
105.90	527.0
108.10	134.0
110.90	116.0
115.90	479.0
116.90	838.0
117.90	357.0
118.80	622.0
127.90	375.0
129.90	228.0
131.00	110.0
135.00	125.0
136.90	224.0
140.90	756.0
142.00	209.0
142.90	1540.0
144.90	717.0
145.80	175.0
148.00	194.0
150.00	145.0
154.80	201.0
170.90	272.0
172.00	765.0
173.00	991.0
174.00	51496.0
175.00	4260.0
176.00	50248.0
177.00	3567.0
177.90	144.0

BEBS34
ClientSampleId :
MS2A047A
Instrument :

m/z	Abundance
36.00	773.0
37.00	3547.0
38.00	3637.0
39.00	1794.0
39.90	410.0
40.70	196.0
41.30	131.0
42.90	163.0
44.00	1136.0
45.00	848.0
46.10	193.0
47.00	1045.0
48.00	436.0
49.00	3336.0
50.00	15598.0
51.10	5087.0
52.10	248.0
52.90	160.0
53.80	193.0
54.80	306.0
56.00	1242.0
57.00	2589.0
57.90	110.0
58.20	108.0
60.00	759.0
61.00	4030.0
62.00	3942.0
63.00	3488.0
64.00	866.0
65.00	825.0
66.80	369.0
68.00	7659.0
69.00	8708.0
70.00	933.0
72.00	699.0
73.00	3465.0
74.00	13428.0
75.00	39856.0
76.00	3623.0
76.90	538.0
77.80	376.0
78.90	5041.0
80.00	1011.0
81.00	5177.0
81.90	995.0
83.00	115.0
86.10	464.0
87.00	3428.0
87.90	3455.0
90.80	361.0
92.10	2651.0
93.00	3892.0
94.00	9686.0
95.00	76864.0
96.10	5245.0
96.90	218.0
102.70	112.0
104.10	353.0
105.20	116.0
105.90	462.0
107.90	117.0
110.80	139.0
115.00	125.0
115.90	446.0
117.00	887.0
117.90	400.0
118.80	681.0
127.90	450.0
129.90	224.0
130.80	170.0
136.90	269.0
140.90	802.0
142.00	183.0
142.90	1690.0
144.90	747.0
145.80	167.0
147.90	231.0
150.10	151.0
155.00	236.0
156.60	113.0
157.10	148.0
170.90	363.0
172.00	892.0
173.00	1011.0
174.00	56048.0
175.00	4409.0
176.00	54168.0
177.00	3835.0
177.90	136.0

BFB234
ClientSampleId :
MS2A047
Instrument :

m/z	Abundance
36.00	647.0
37.00	3265.0
38.00	3426.0
39.10	1668.0
40.00	397.0
41.10	205.0
42.90	173.0
43.90	1109.0
45.00	790.0
45.90	179.0
46.90	992.0
48.00	355.0
49.00	3196.0
50.00	14556.0
51.10	4860.0
52.10	281.0
52.90	171.0
53.80	206.0
54.90	321.0
56.00	1410.0
57.00	2561.0
57.90	159.0
60.00	747.0
61.00	4008.0
62.00	3801.0
63.10	3178.0
64.00	877.0
65.00	831.0
66.90	388.0
68.00	7351.0
69.10	8236.0
70.00	850.0
72.00	669.0
73.00	3306.0
74.10	12564.0
75.00	37904.0
76.00	3549.0
76.90	510.0
78.00	372.0
78.90	4812.0
80.00	960.0
81.00	4841.0
81.90	1010.0
83.00	137.0
86.20	419.0
87.00	3324.0
88.00	3067.0
90.80	354.0
92.10	2291.0
93.00	3890.0
94.00	9550.0
95.00	71880.0
96.10	4904.0
104.10	318.0
104.70	134.0
105.20	122.0
105.90	356.0
107.80	164.0
110.80	149.0
115.00	118.0
115.90	312.0
117.00	871.0
117.90	416.0
118.80	694.0
127.90	477.0
128.80	103.0
129.80	271.0
130.80	229.0
136.90	290.0
140.90	724.0
142.00	148.0
142.90	1774.0
144.90	708.0
145.70	138.0
146.20	104.0
147.90	237.0
150.10	118.0
152.90	101.0
155.10	232.0
156.70	108.0
157.20	148.0
160.80	123.0
170.90	381.0
172.00	896.0
173.00	970.0
174.00	55880.0
175.00	4016.0
176.00	53112.0
177.00	3668.0
177.90	139.0

BFB234
ClientSampleId :
MS2A047
Instrument :