
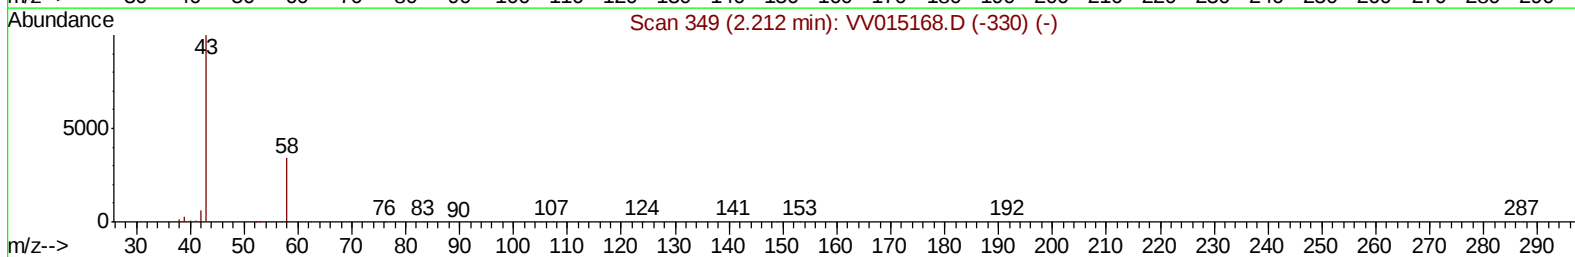
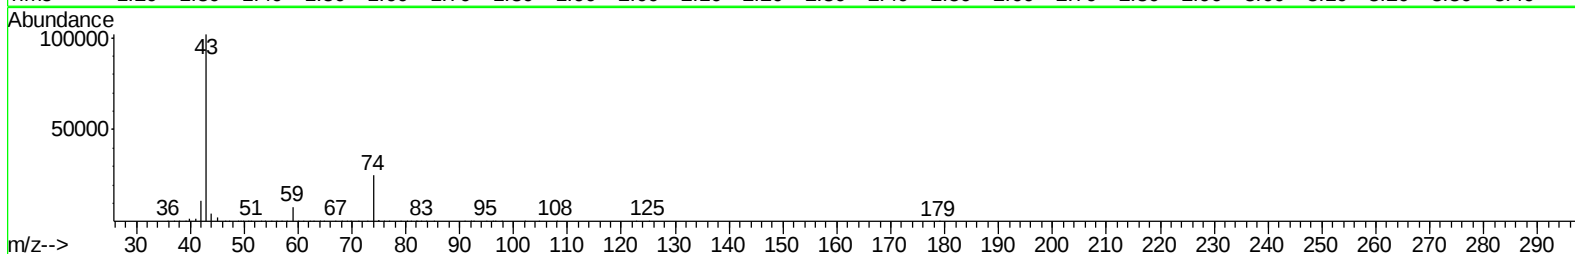


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015172.D
 Acq On : 26 Mar 2020 17:33
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 03:05:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 26 19:04:37 2020
 Response via : Initial Calibration

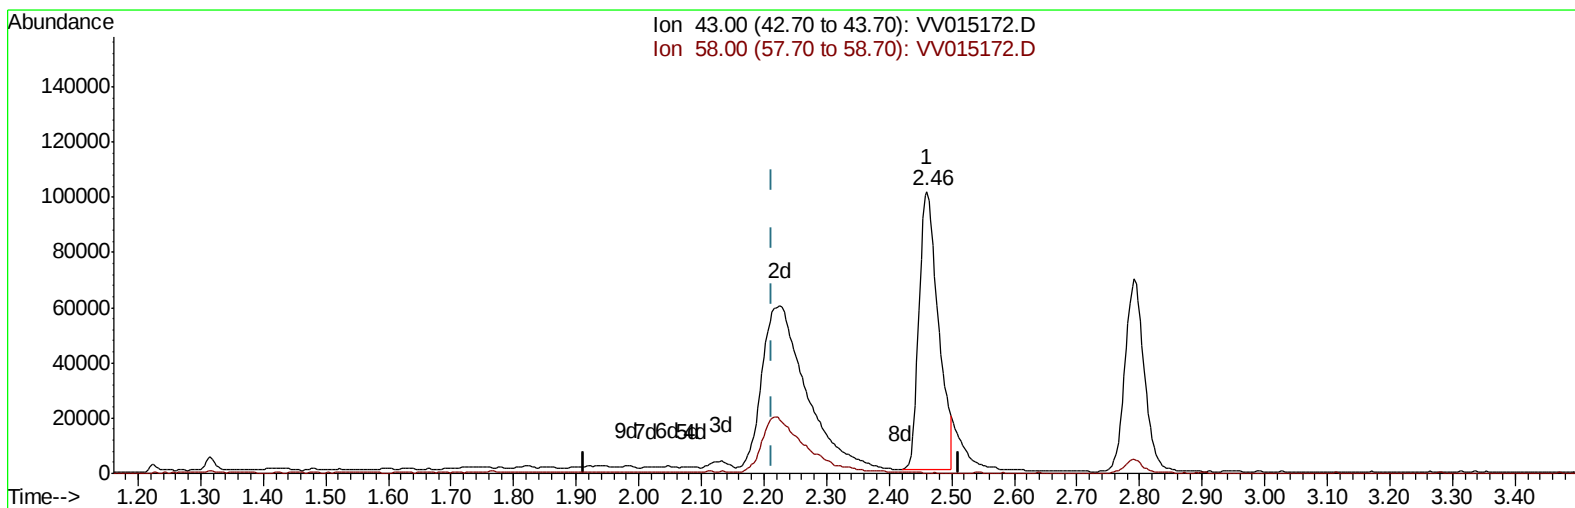

TIC: VV015172.D

(13) Acetone (T)

2.460min (+0.248) 83.33ug/L

response 217425

Ion	Exp%	Act%
43.00	100	100
58.00	0.10	0.01
0.00	0.00	0.00
0.00	0.00	0.00