
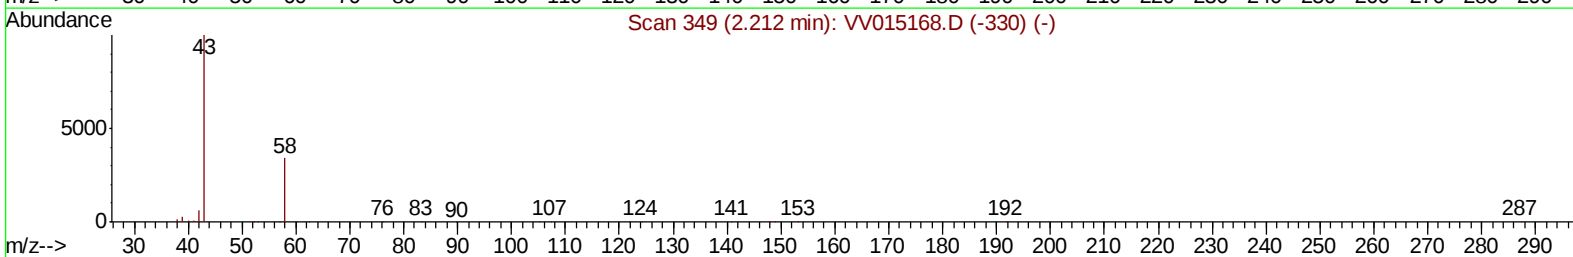
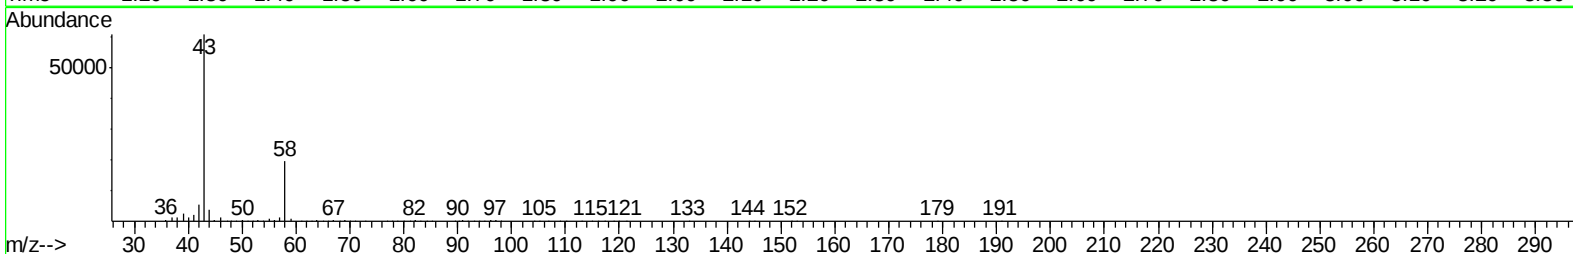


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015172.D
Acq On : 26 Mar 2020 17:33
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 03:05:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 26 19:04:37 2020
Response via : Initial Calibration

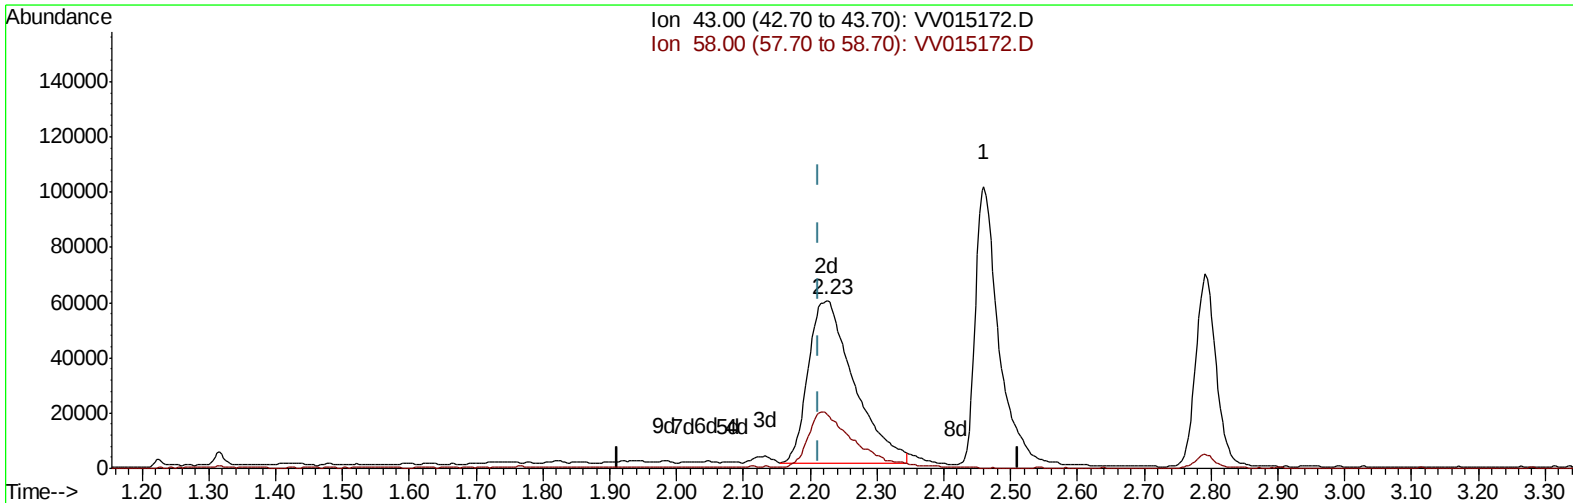

TIC: VV015172.D

(13) Acetone (T)

2.225min (+0.013) 108.21ug/L m

response 282343

Ion	Exp%	Act%
43.00	100	100
58.00	0.10	0.00
0.00	0.00	0.00
0.00	0.00	0.00