
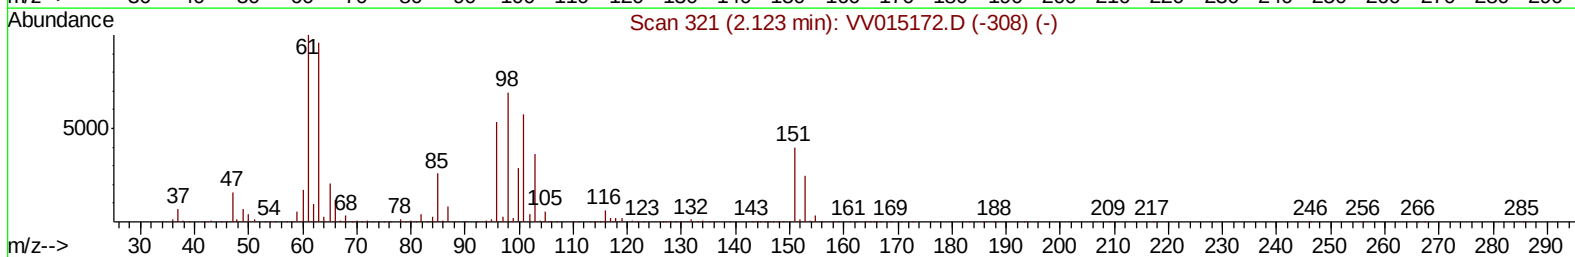
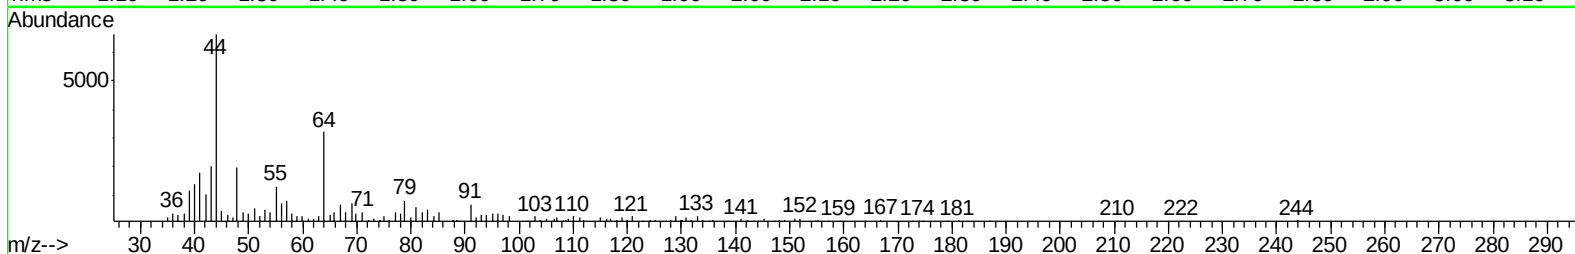


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015181.D
 Acq On : 26 Mar 2020 21:48
 Operator : SY/MD
 Sample : VIBLK72
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 03:40:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 27 03:08:32 2020
 Response via : Initial Calibration

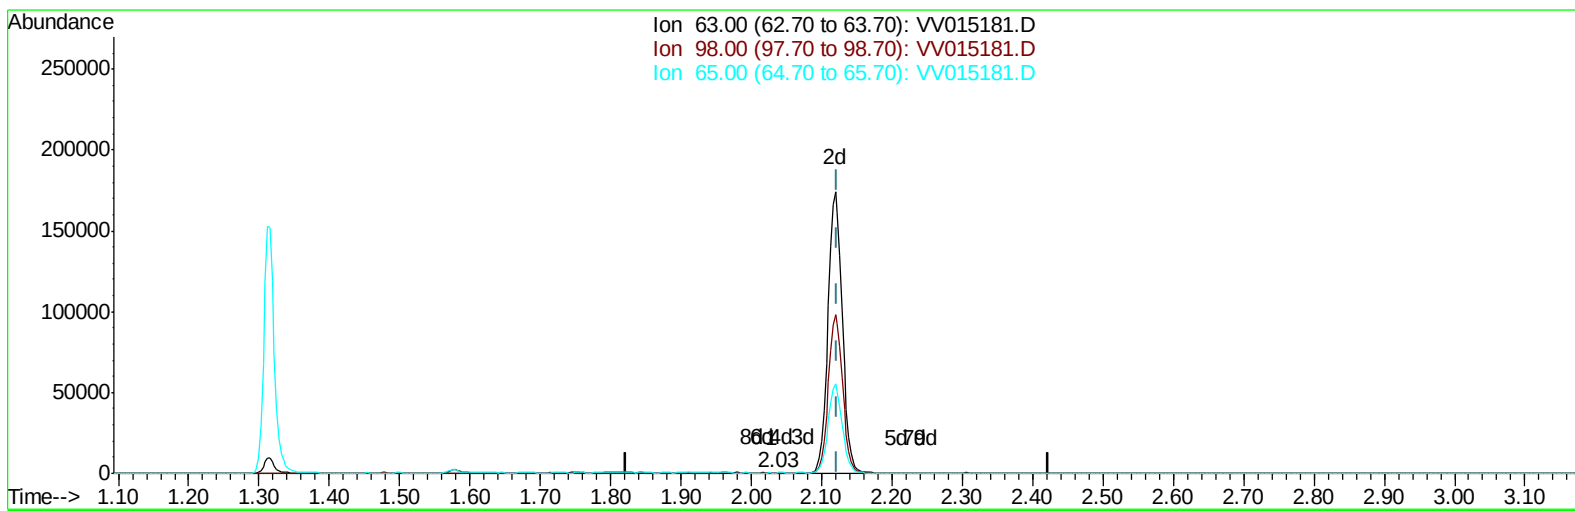

TIC: VV015181.D

(11) 1,1-Dichloroethene-d2 (S)

2.029min (-0.093) 0.03ug/L

response 250

Ion	Exp%	Act%
63.00	100	100
98.00	75.60	70.80
65.00	20.40	25.60
0.00	0.00	0.00