
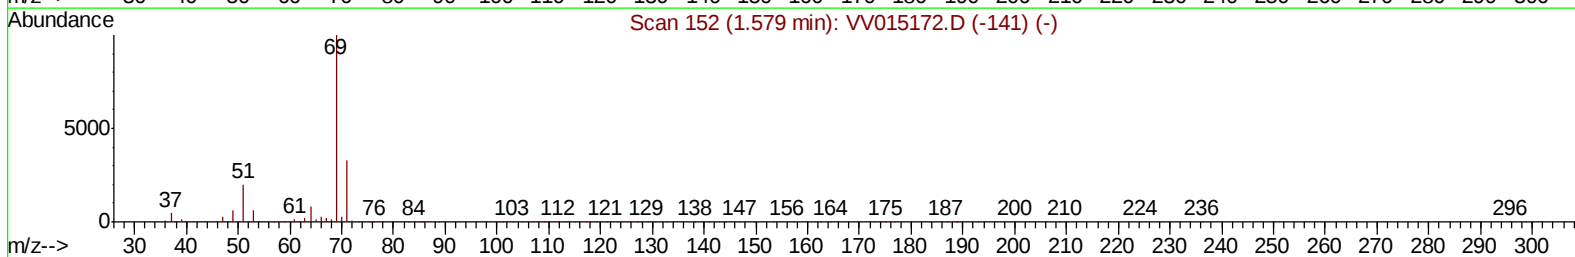
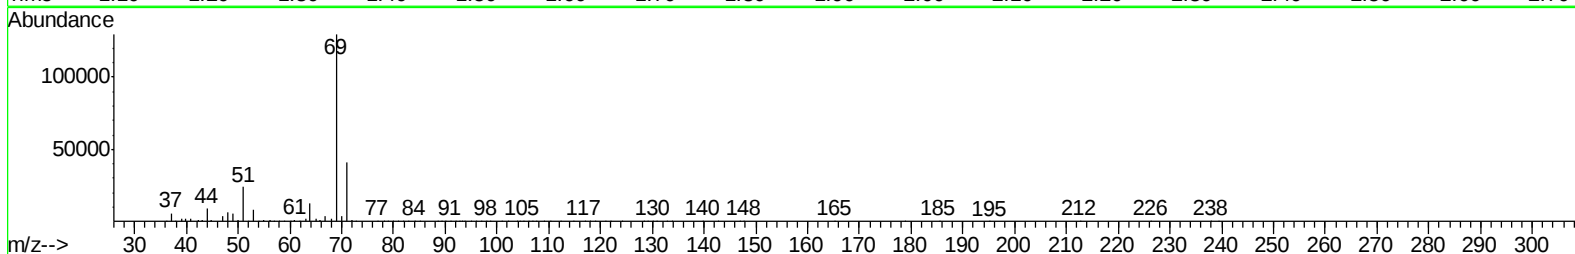


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015181.D
Acq On : 26 Mar 2020 21:48
Operator : SY/MD
Sample : VIBLK72
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 03:40:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 27 03:08:32 2020
Response via : Initial Calibration

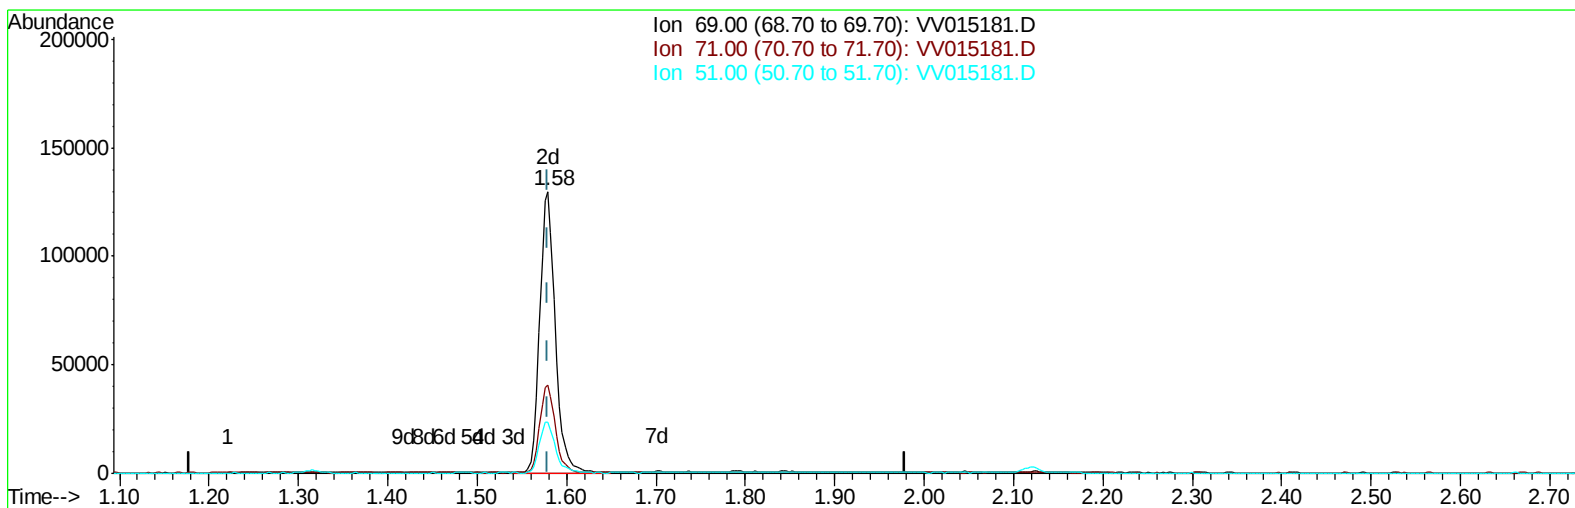

TIC: VV015181.D

(7) Chloroethane-d5 (S)

1.579min (-0.000) 43.30ug/L m

response 157287

Ion	Exp%	Act%
69.00	100	100
71.00	31.40	0.04#
51.00	28.10	0.03#
0.00	0.00	0.00