
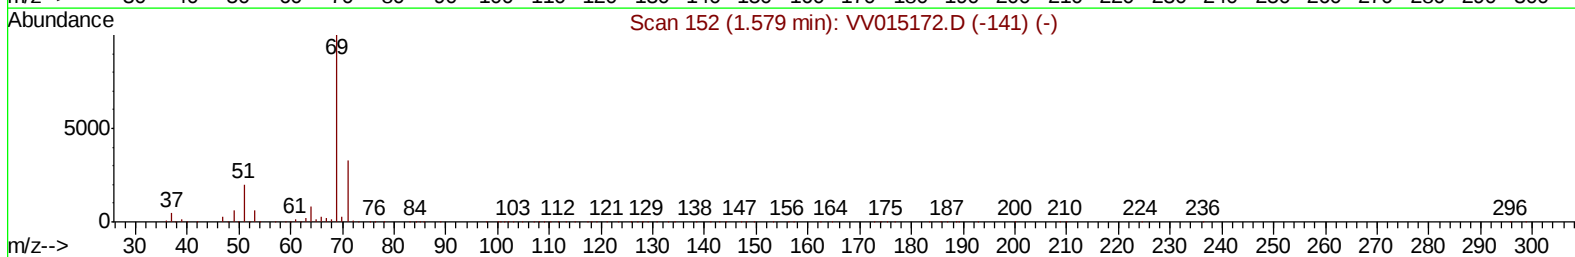
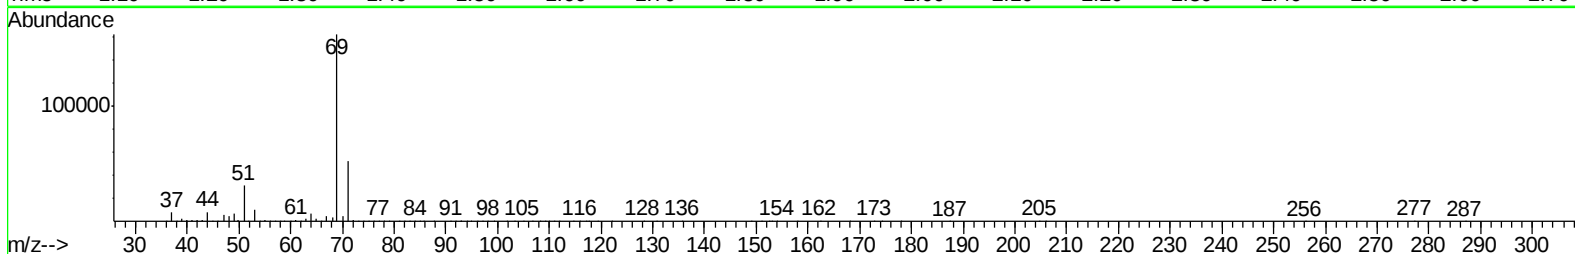


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015182.D
 Acq On : 26 Mar 2020 22:12
 Operator : SY/MD
 Sample : L1968-16 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 03:40:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 27 03:08:32 2020
 Response via : Initial Calibration

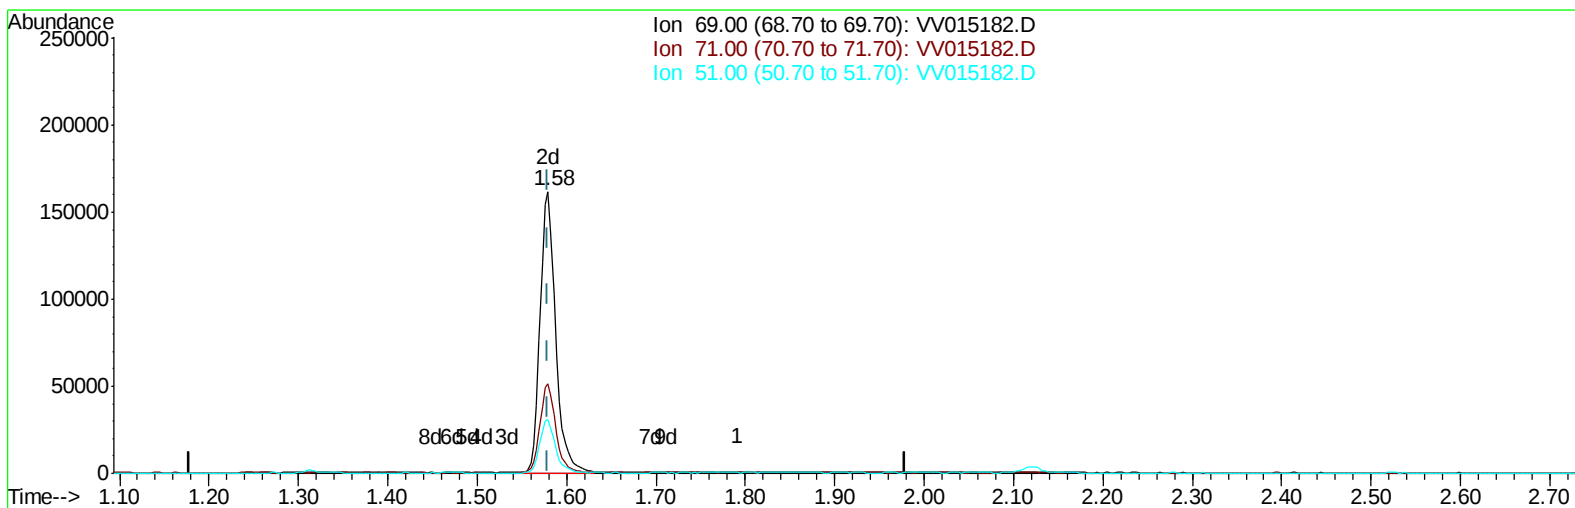

TIC: VV015182.D

(7) Chloroethane-d5 (S)

1.579min (-0.000) 61.66ug/L m

response 196128

Ion	Exp%	Act%
69.00	100	100
71.00	31.40	0.11#
51.00	28.10	0.09#
0.00	0.00	0.00