
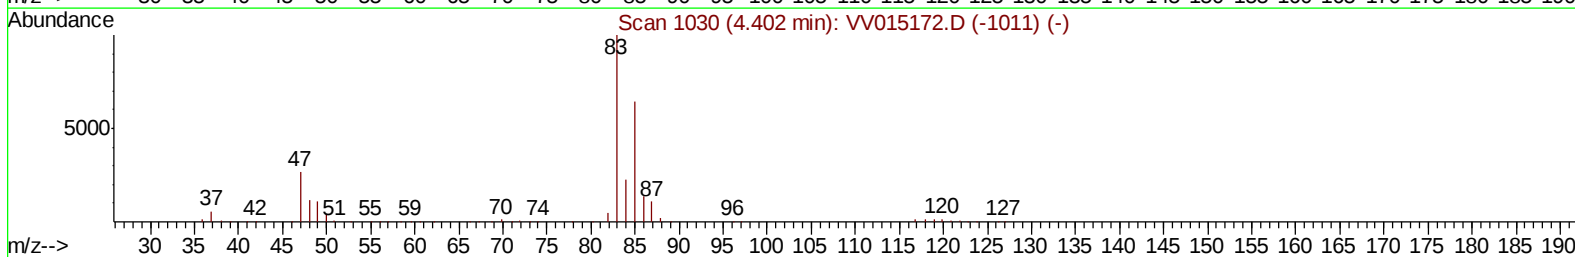
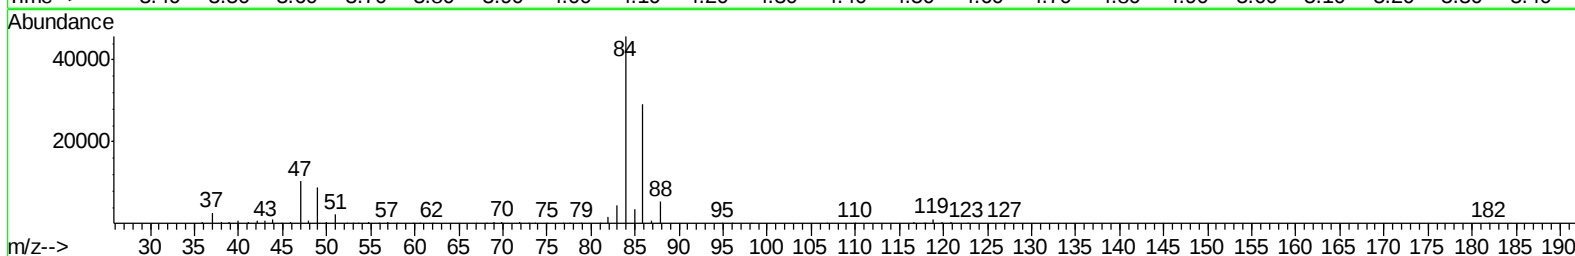


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015184.D
Acq On : 26 Mar 2020 23:01
Operator : SY/MD
Sample : VIBLK73
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 03:40:41 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 27 03:08:32 2020
Response via : Initial Calibration

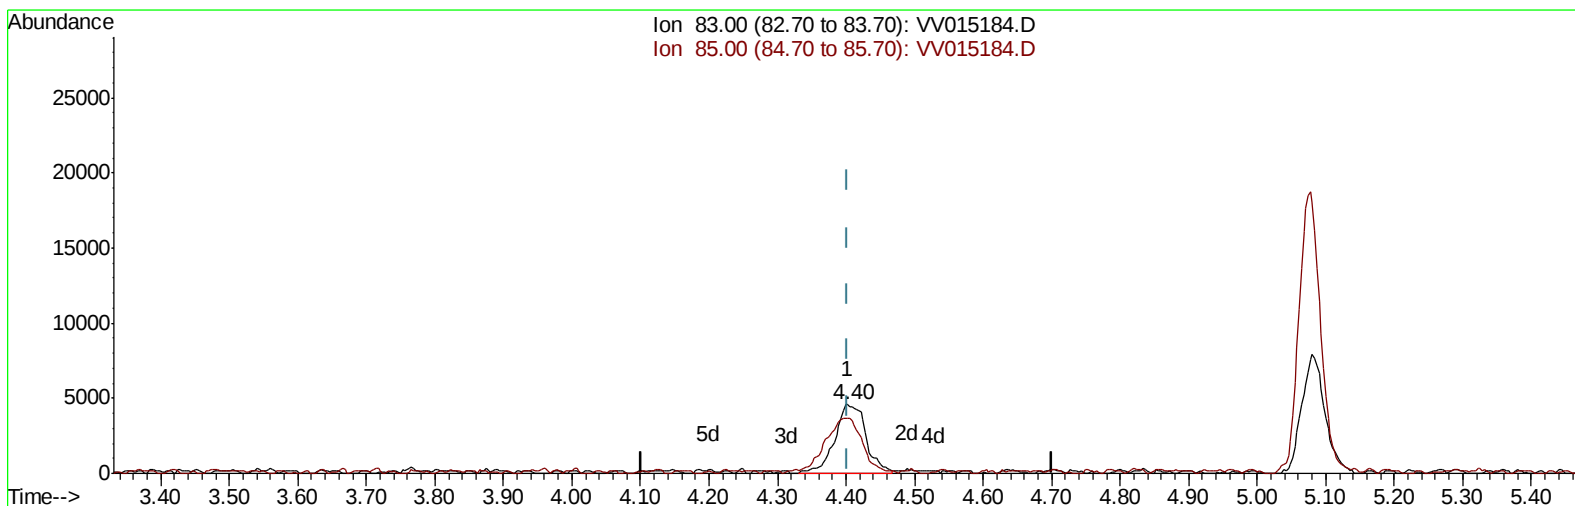

TIC: VV015184.D

(25) Chloroform (T)

4.402min (+0.000) 1.75ug/L m

response 14571

Ion	Exp%	Act%
83.00	100	100
85.00	66.00	80.75
0.00	0.00	0.00
0.00	0.00	0.00