
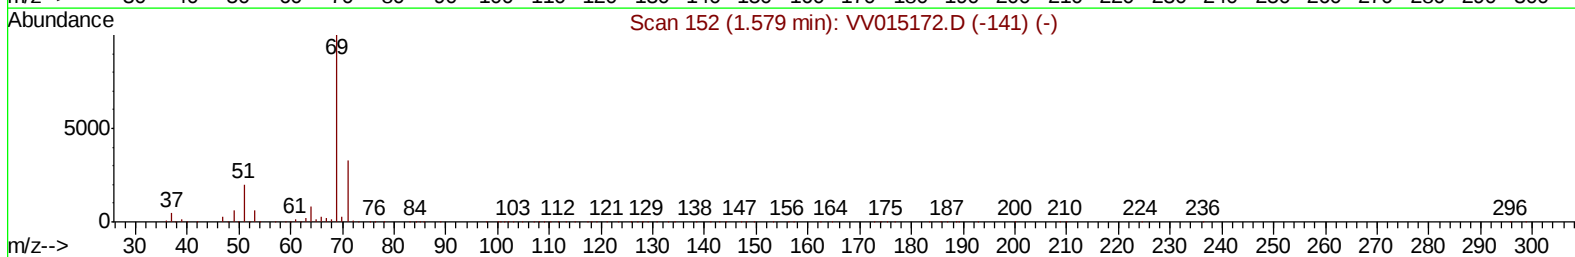
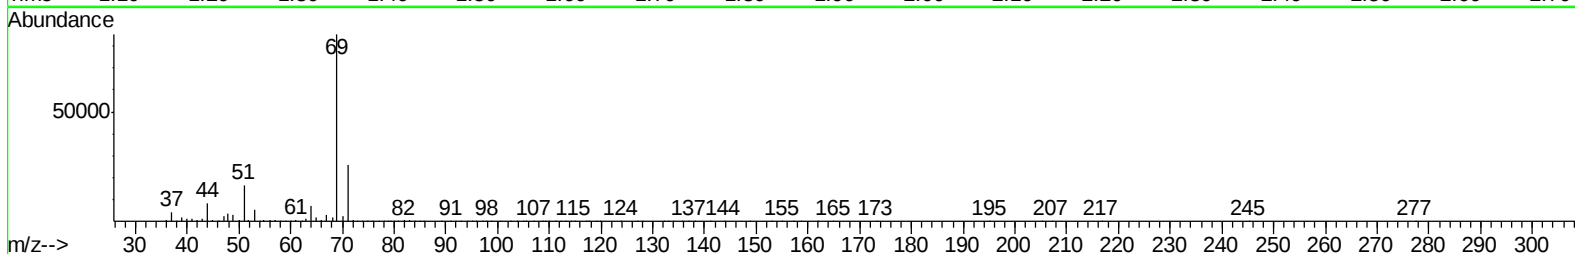


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015186.D
Acq On : 26 Mar 2020 23:49
Operator : SY/MD
Sample : L1976-02MS
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 03:40:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 27 03:08:32 2020
Response via : Initial Calibration

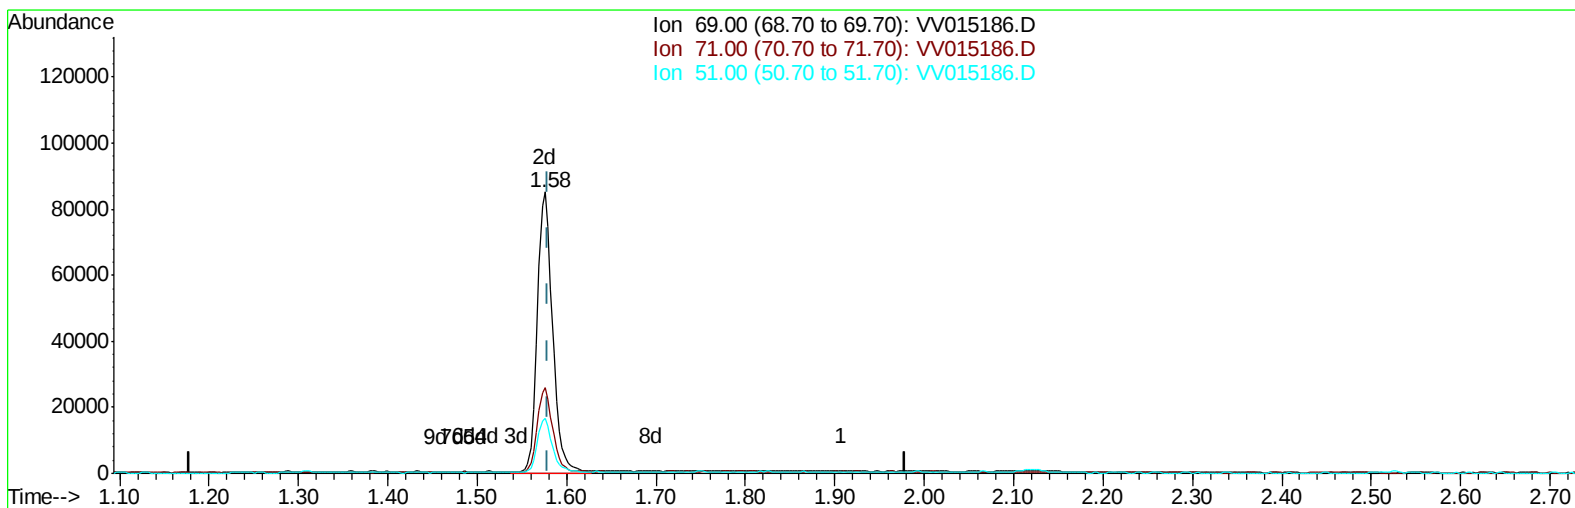

TIC: VV015186.D

(7) Chloroethane-d5 (S)

1.576min (-0.003) 70.84ug/L m

response 102089

Ion	Exp%	Act%
69.00	100	100
71.00	31.40	0.10#
51.00	28.10	0.10#
0.00	0.00	0.00