
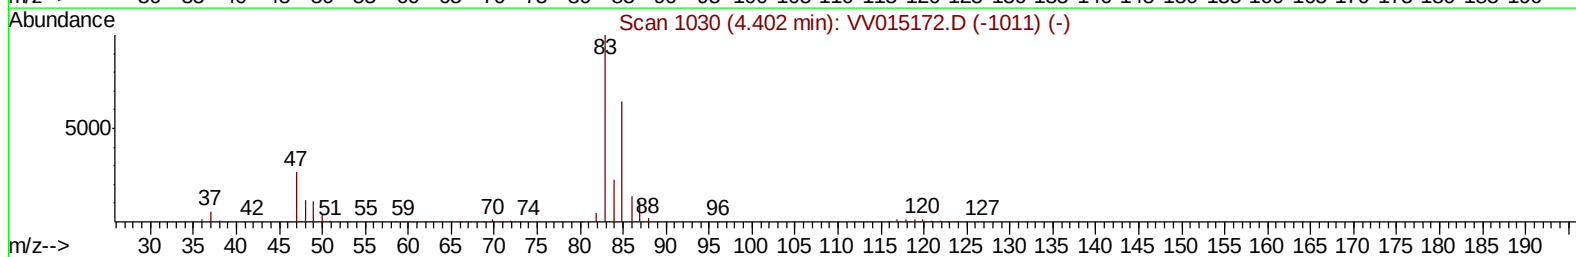
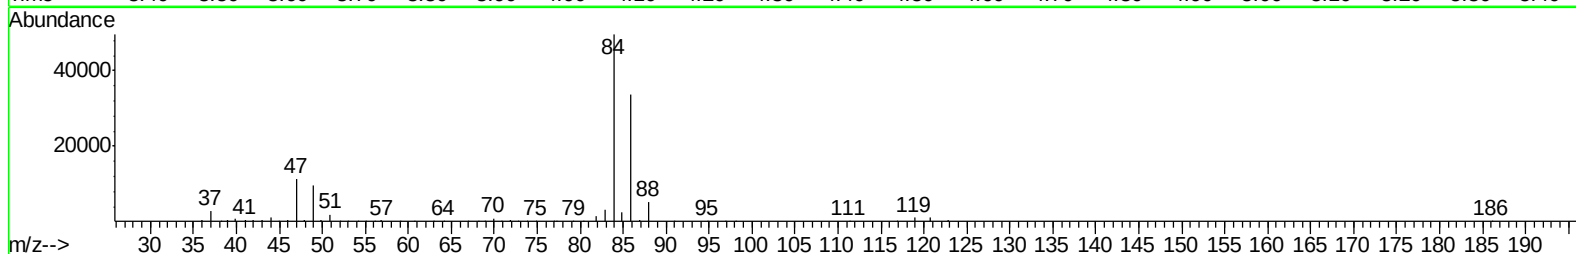


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015187.D
Acq On : 27 Mar 2020 00:14
Operator : SY/MD
Sample : L1976-03MSD
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 03:41:08 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 27 03:08:32 2020
Response via : Initial Calibration

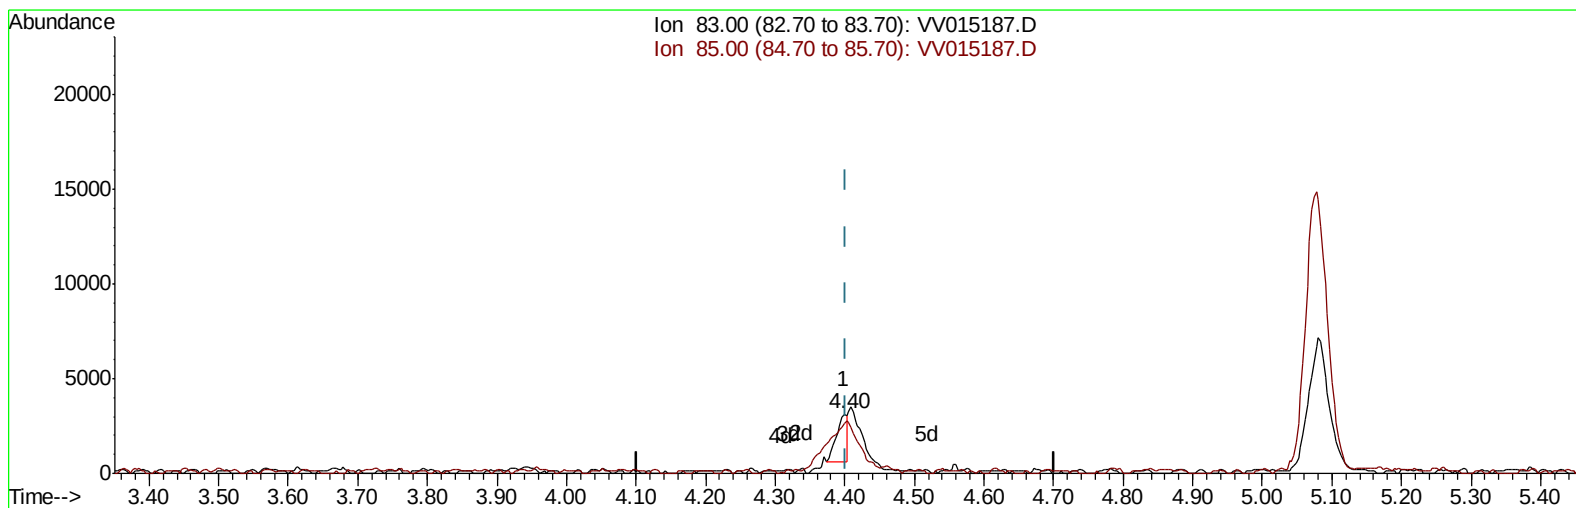

TIC: VV015187.D

(25) Chloroform (T)

4.399min (-0.003) 0.43ug/L

response 2592

Ion	Exp%	Act%
83.00	100	100
85.00	66.00	83.13
0.00	0.00	0.00
0.00	0.00	0.00