
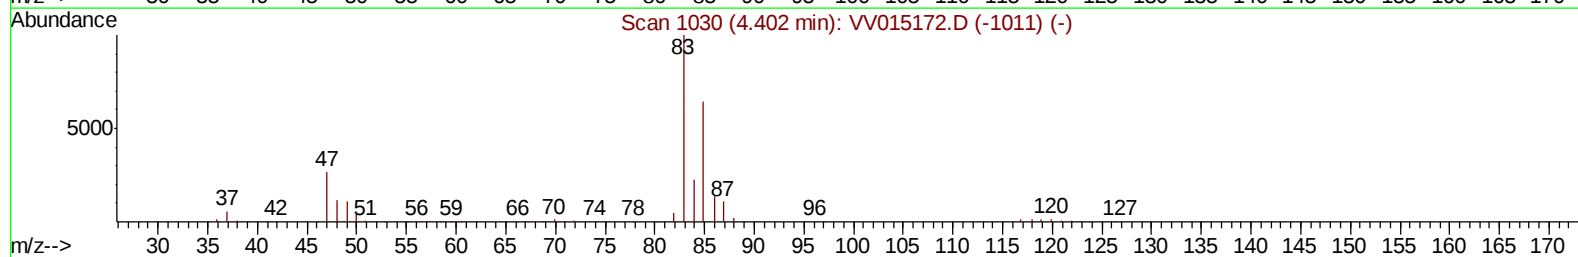
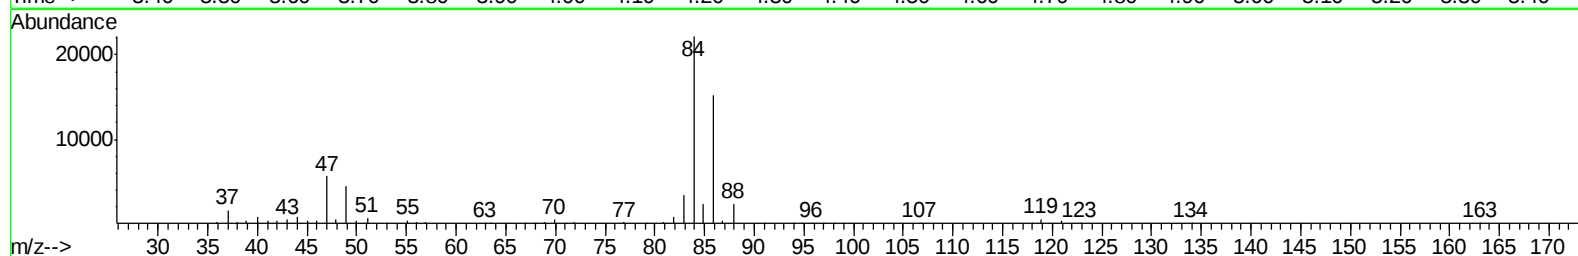


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015187.D
 Acq On : 27 Mar 2020 00:14
 Operator : SY/MD
 Sample : L1976-03MSD
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 03:41:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 27 03:08:32 2020
 Response via : Initial Calibration

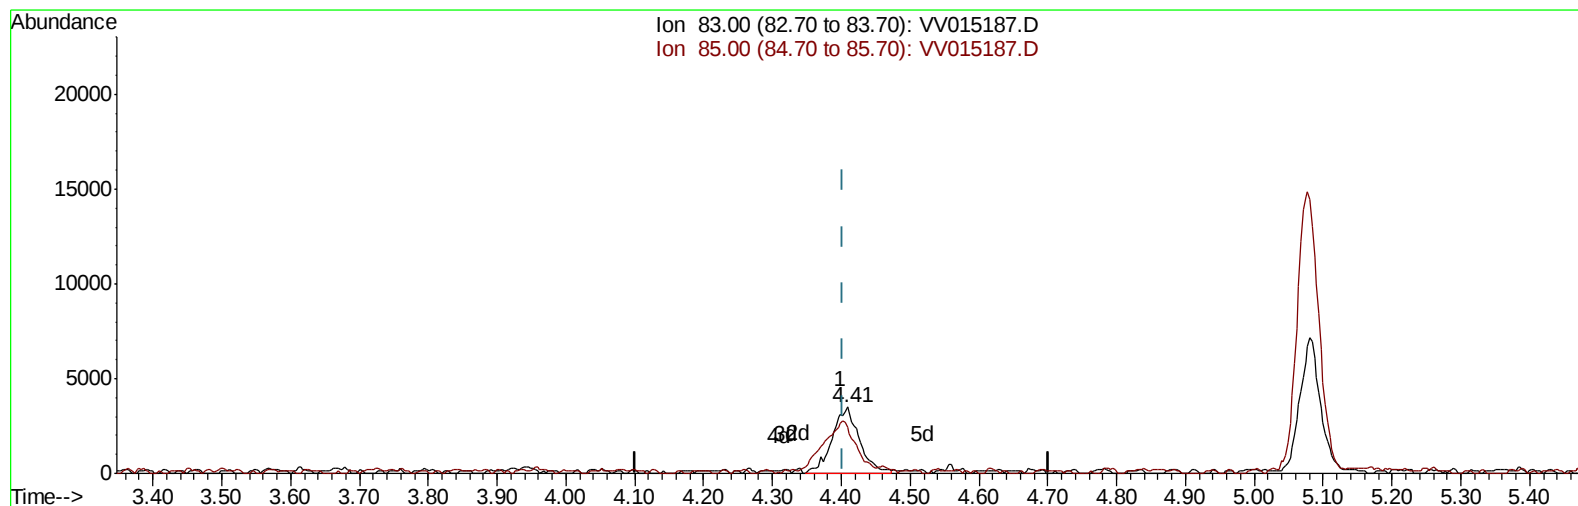

TIC: VV015187.D

(25) Chloroform (T)

4.409min (+0.006) 1.62ug/L m

response 9684

Ion	Exp%	Act%
83.00	100	100
85.00	66.00	69.16
0.00	0.00	0.00
0.00	0.00	0.00