
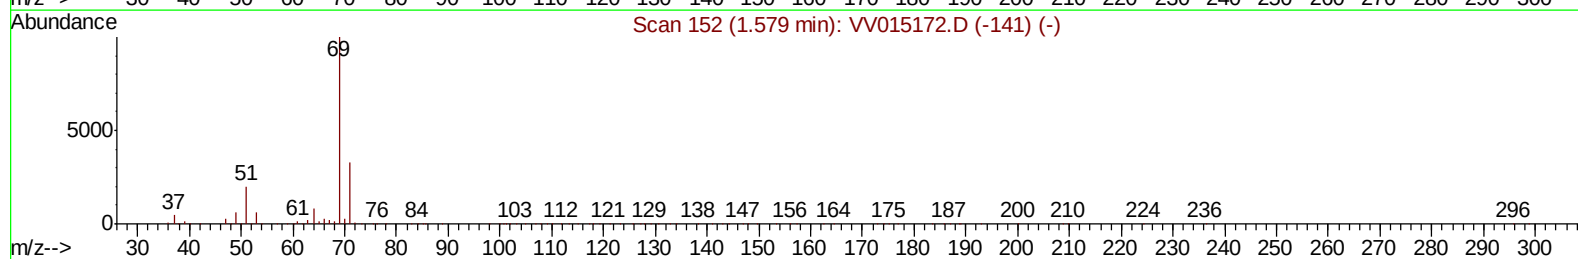
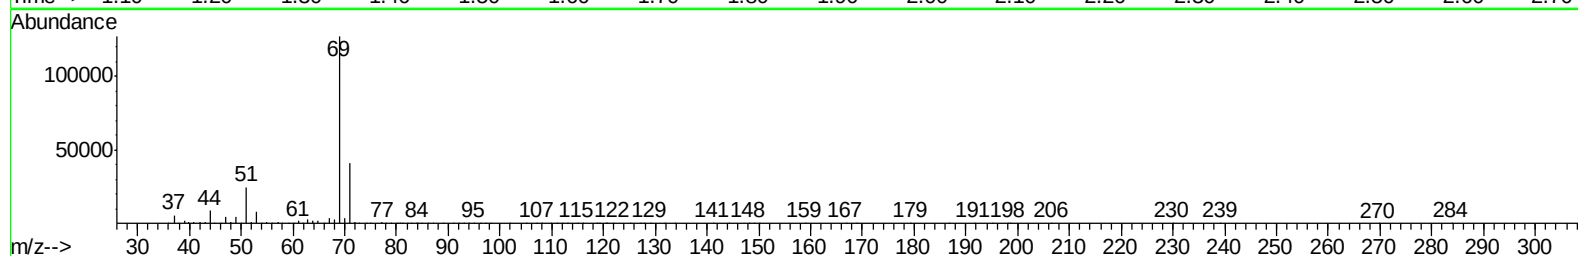


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015192.D
 Acq On : 27 Mar 2020 02:15
 Operator : SY/MD
 Sample : L1976-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 03:41:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 27 03:08:32 2020
 Response via : Initial Calibration

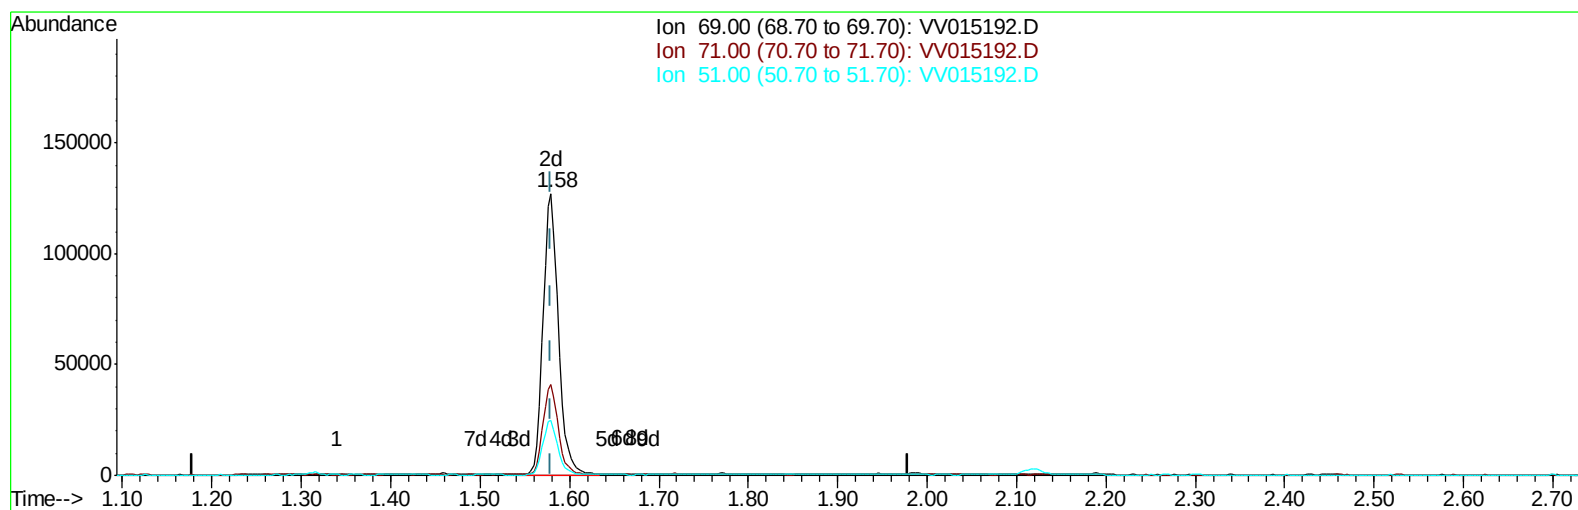

TIC: VV015192.D

(7) Chloroethane-d5 (S)

1.579min (+0.000) 50.84ug/L m

response 151833

Ion	Exp%	Act%
69.00	100	100
71.00	31.40	0.04#
51.00	28.10	0.04#
0.00	0.00	0.00