
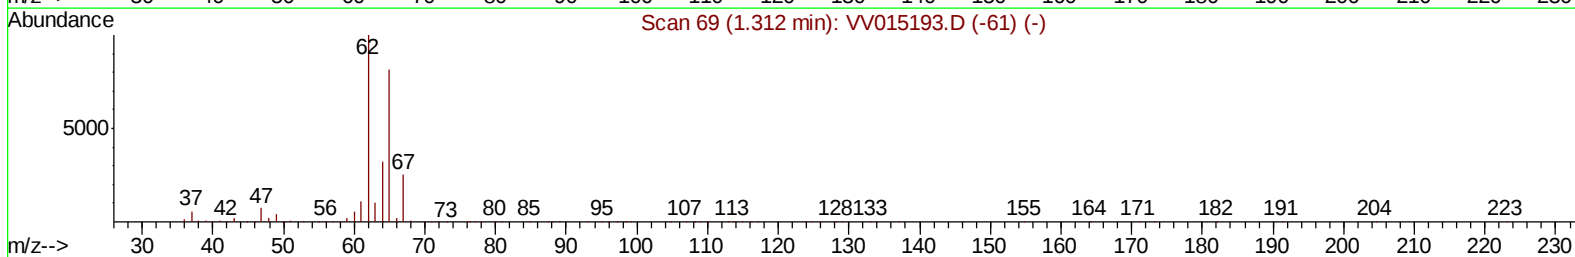
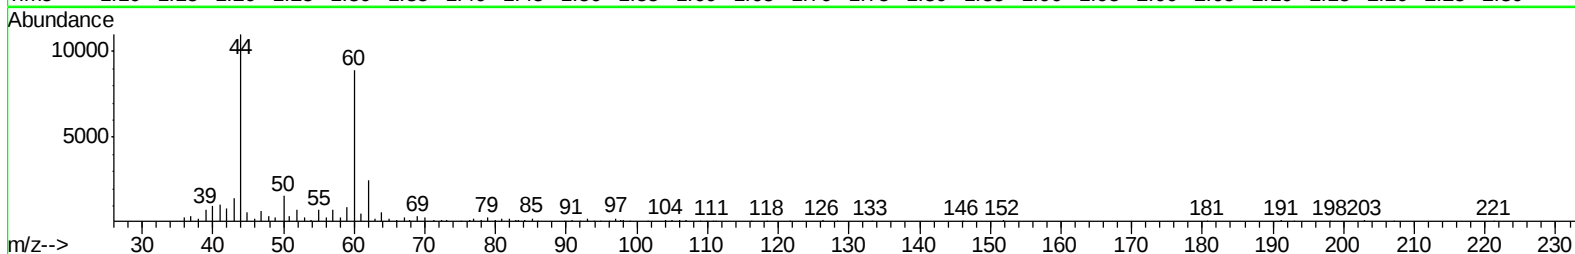


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015196.D
 Acq On : 27 Mar 2020 05:46
 Operator : SY/MD
 Sample : L1976-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 07:37:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 27 06:56:02 2020
 Response via : Initial Calibration

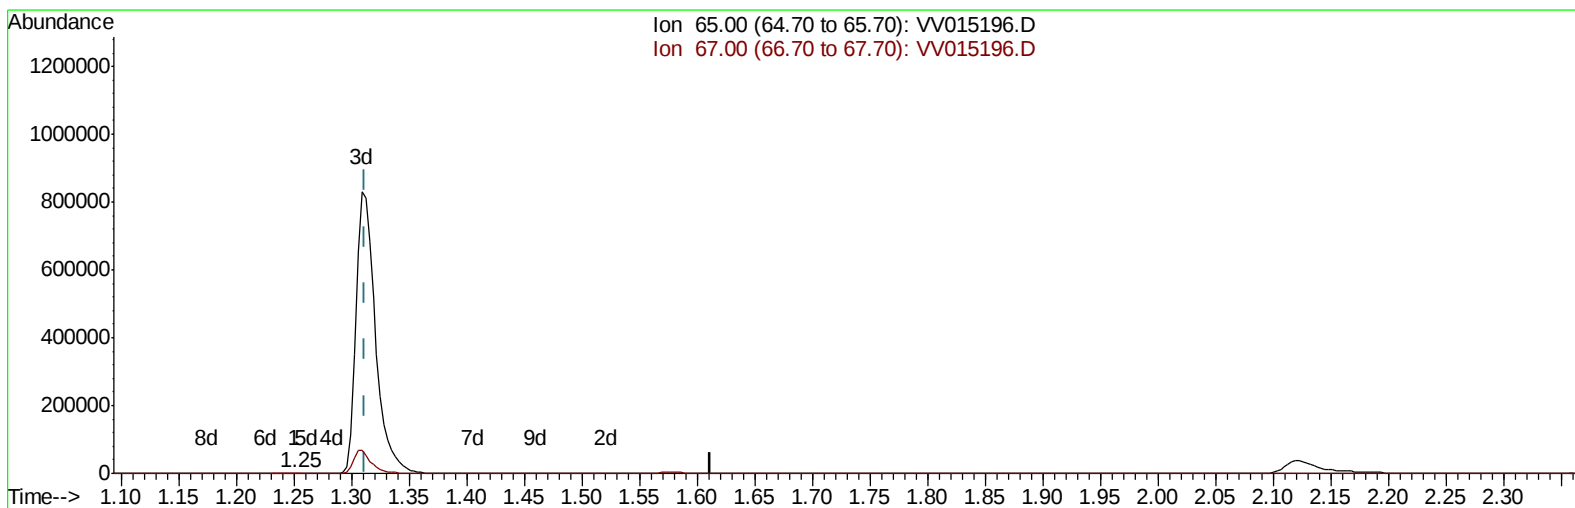

TIC: VV015196.D

(4) Vinyl Chloride-d3 (S)

1.251min (-0.061) 0.04ug/L

response 144

Ion	Exp%	Act%
65.00	100	100
67.00	32.70	31.94
0.00	0.00	0.00
0.00	0.00	0.00