
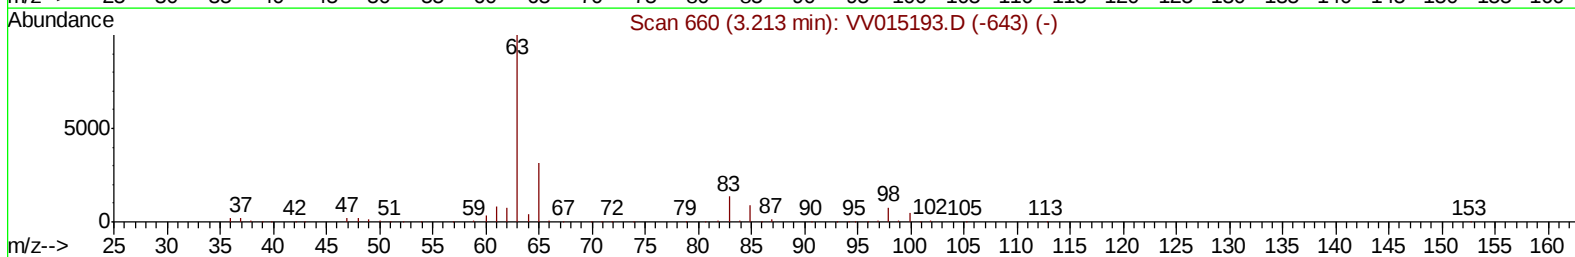
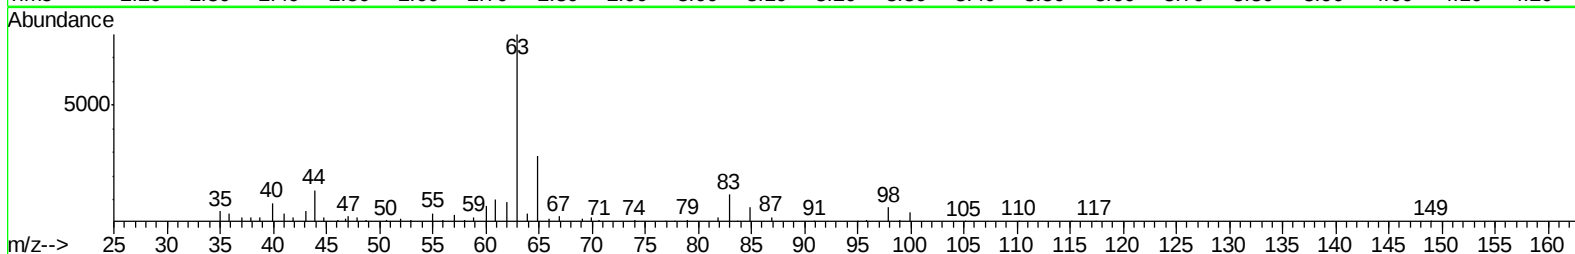


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015196.D
Acq On : 27 Mar 2020 05:46
Operator : SY/MD
Sample : L1976-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 07:37:00 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 27 06:56:02 2020
Response via : Initial Calibration

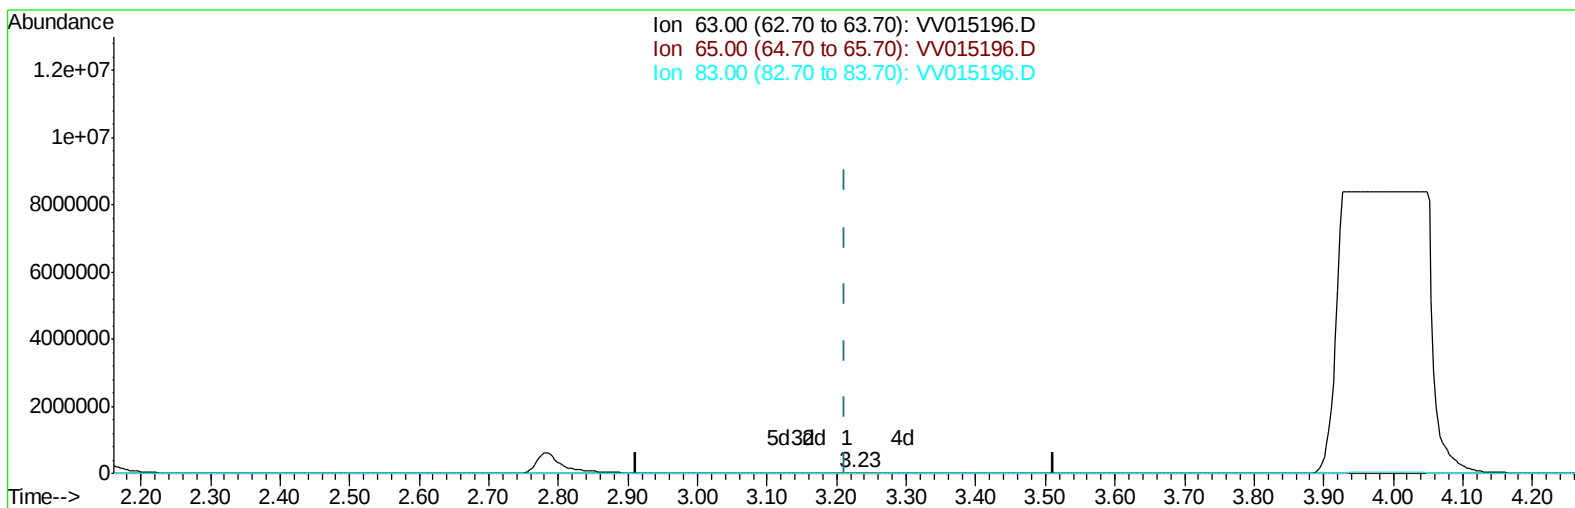

TIC: VV015196.D

(19) 1,1-Dichloroethane (T)

3.225min (+0.013) 2.09ug/L m

response 19728

Ion	Exp%	Act%
63.00	100	100
65.00	31.70	35.58
83.00	13.70	15.35
0.00	0.00	0.00