
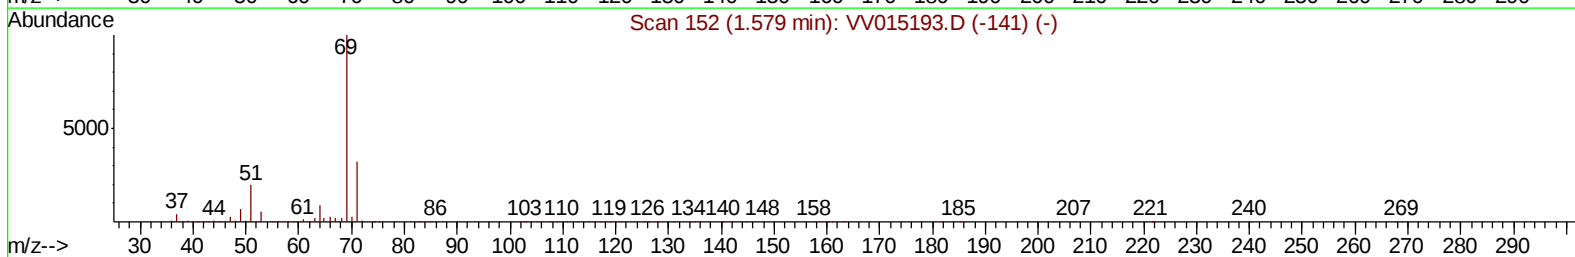
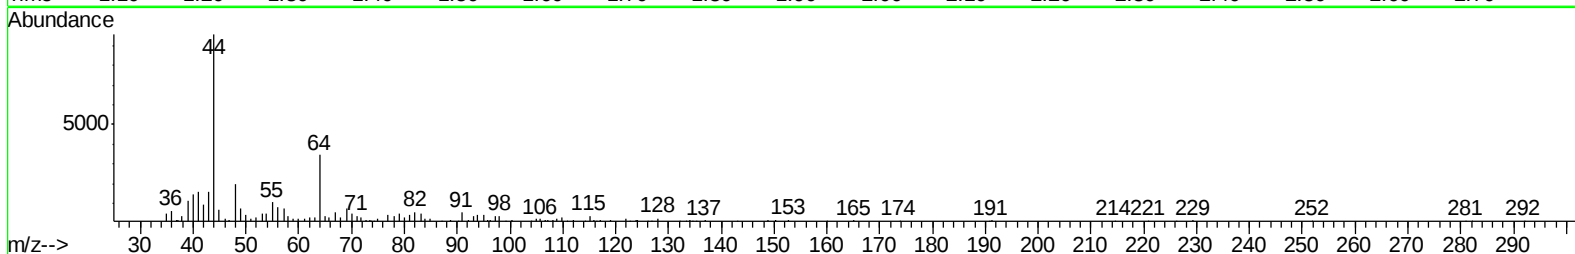


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015200.D
Acq On : 27 Mar 2020 09:38
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 01:38:54 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 28 01:31:46 2020
Response via : Initial Calibration

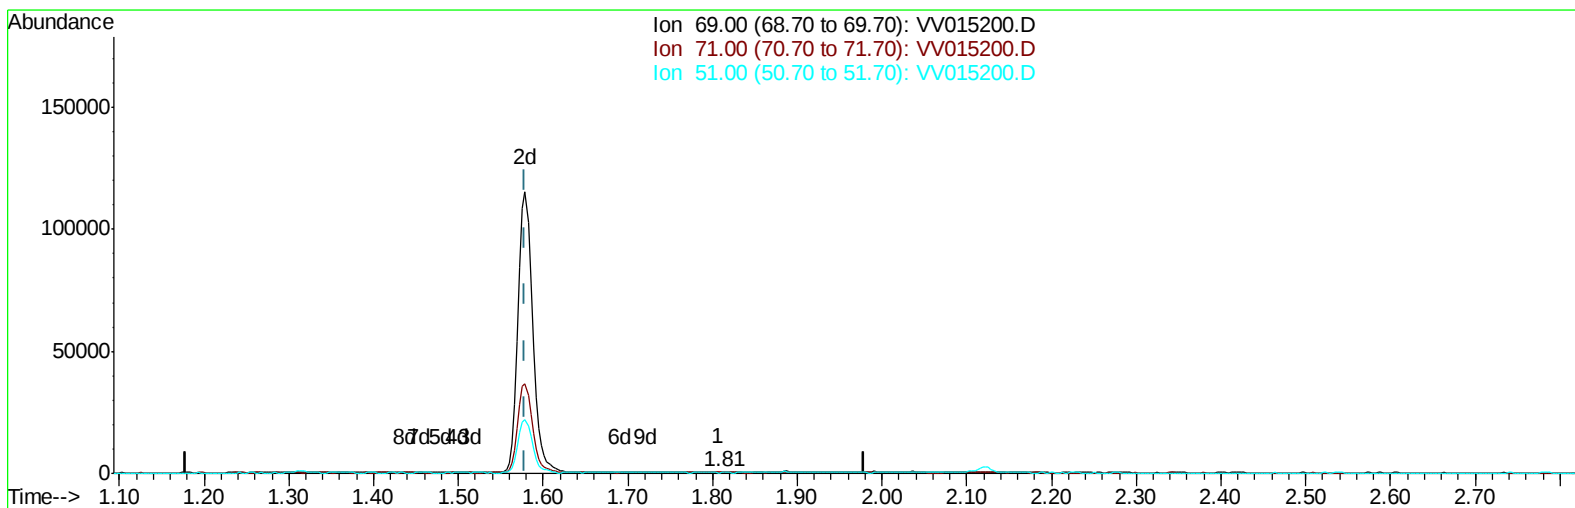

TIC: VV015200.D

(7) Chloroethane-d5 (S)

1.807min (+0.228) 0.13ug/L

response 434

Ion	Exp%	Act%
69.00	100	100
71.00	31.40	30.18
51.00	28.10	21.66
0.00	0.00	0.00