
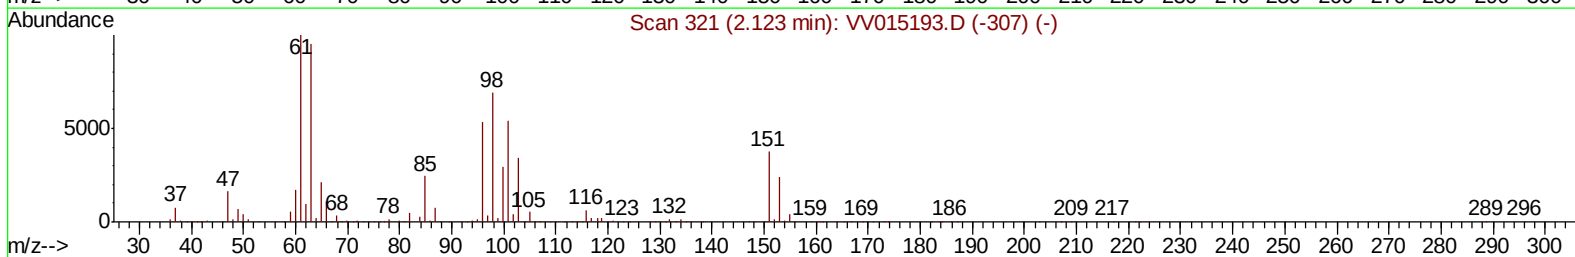
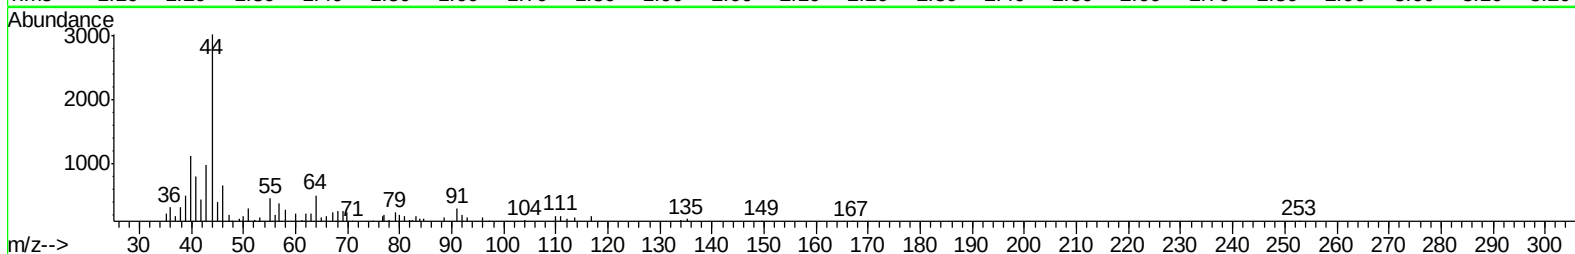


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015200.D
Acq On : 27 Mar 2020 09:38
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 01:38:54 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 28 01:31:46 2020
Response via : Initial Calibration

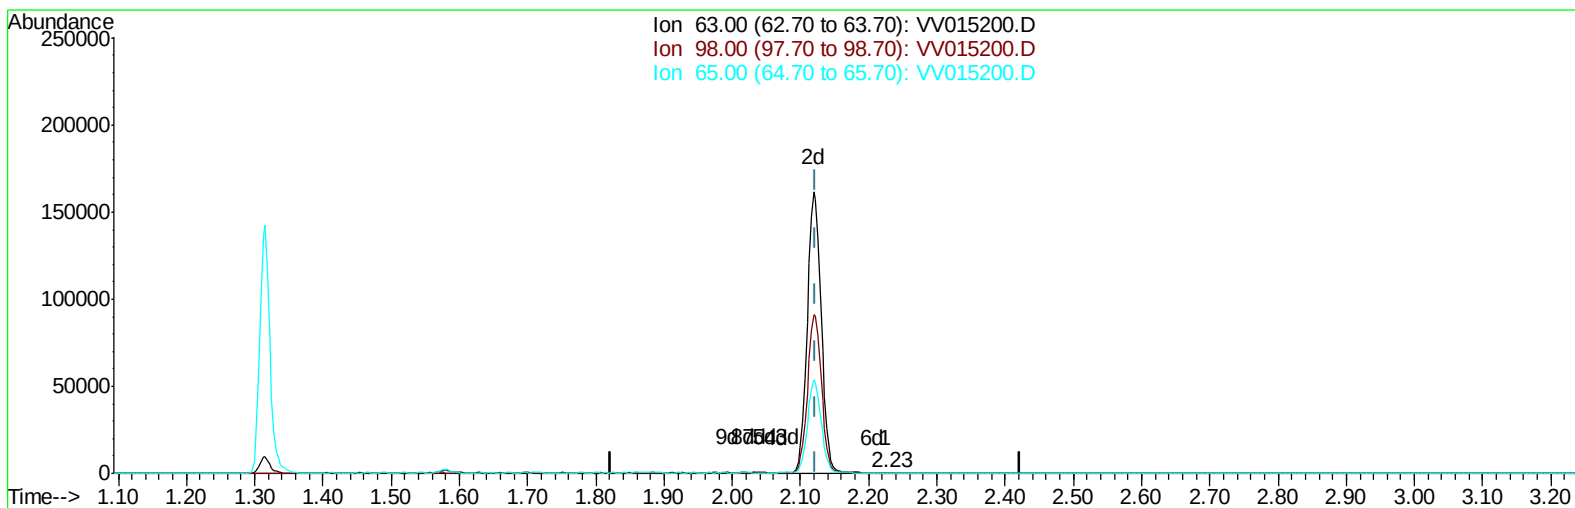

TIC: VV015200.D

(11) 1,1-Dichloroethene-d2 (S)

2.225min (+0.103) 0.03ug/L

response 248

Ion	Exp%	Act%
63.00	100	100
98.00	75.60	90.32
65.00	20.40	24.60
0.00	0.00	0.00