
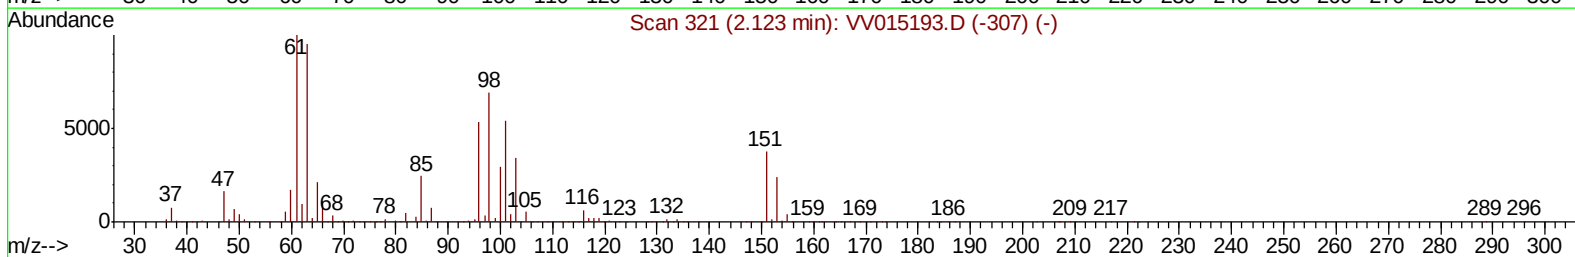
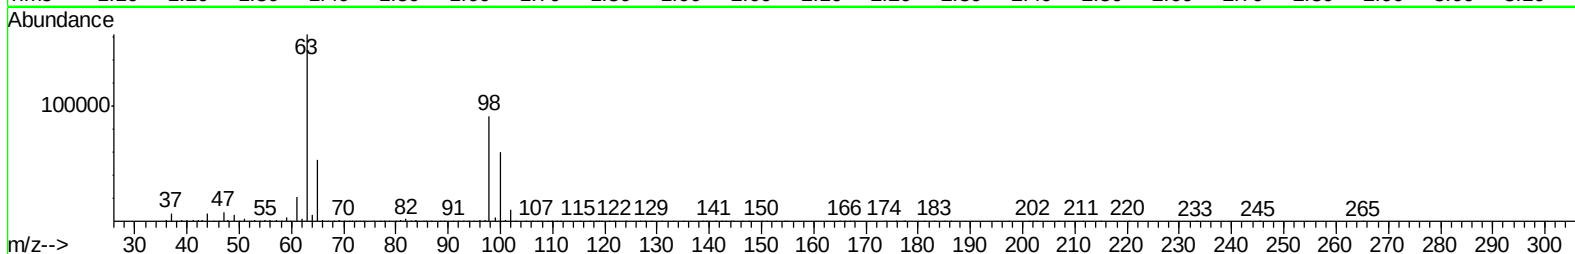


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015200.D
 Acq On : 27 Mar 2020 09:38
 Operator : SY/MD
 Sample : VIBLK74
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 01:38:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 01:31:46 2020
 Response via : Initial Calibration

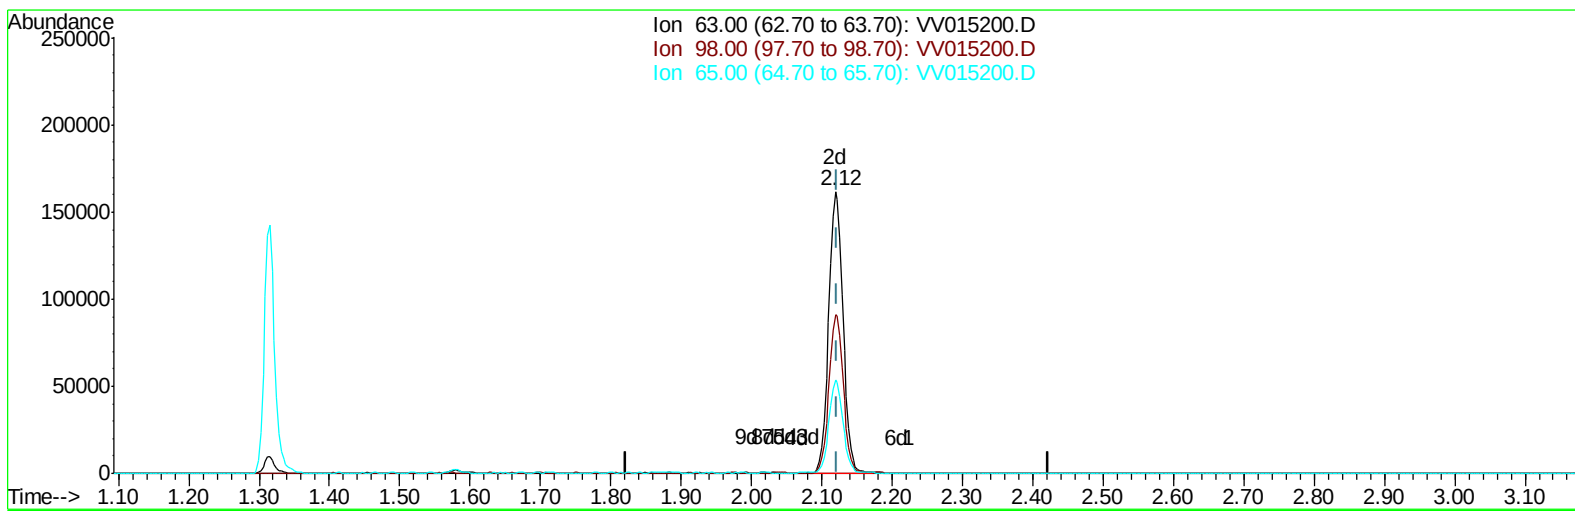

TIC: VV015200.D

(11) 1,1-Dichloroethene-d2 (S)

2.119min (-0.003) 31.49ug/L m

response 230902

Ion	Exp%	Act%
63.00	100	100
98.00	75.60	0.10#
65.00	20.40	0.03#
0.00	0.00	0.00