
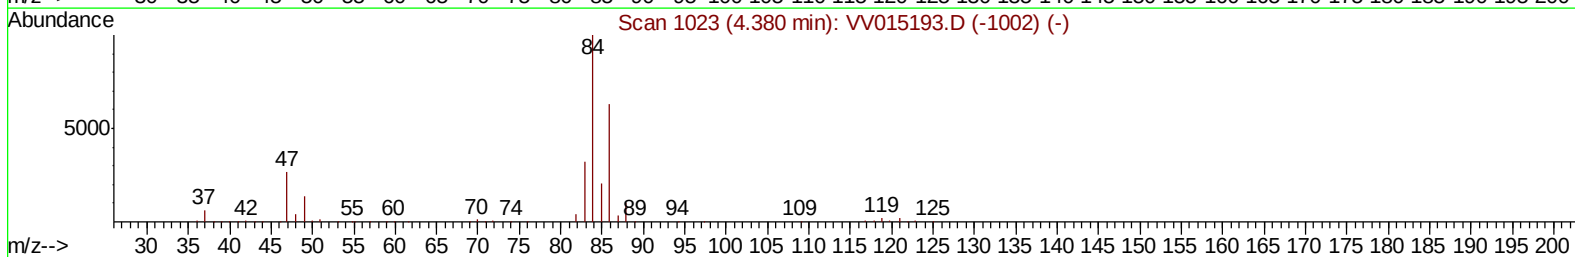
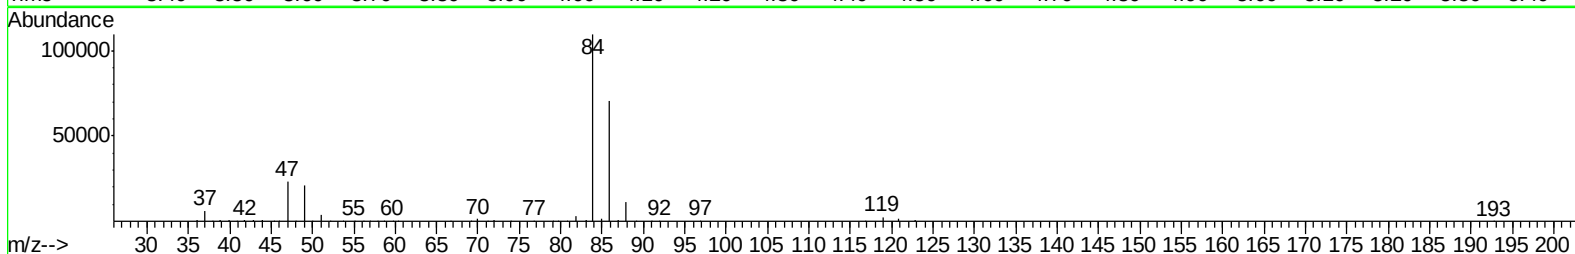


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015203.D
 Acq On : 27 Mar 2020 10:58
 Operator : SY/MD
 Sample : L1976-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 01:39:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 01:31:46 2020
 Response via : Initial Calibration

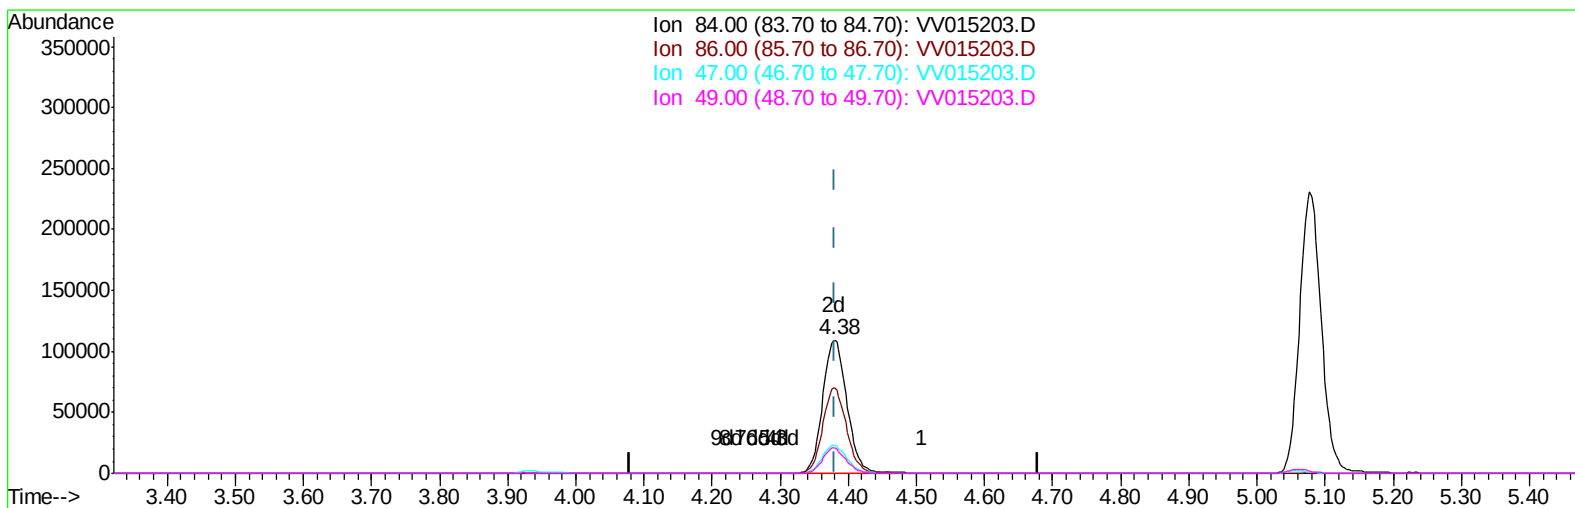

TIC: VV015203.D

(24) Chloroform-d (S)

4.380min (-0.000) 45.53ug/L m

response 268530

Ion	Exp%	Act%
84.00	100	100
86.00	61.90	0.07#
47.00	44.80	0.05#
49.00	26.30	0.02#