
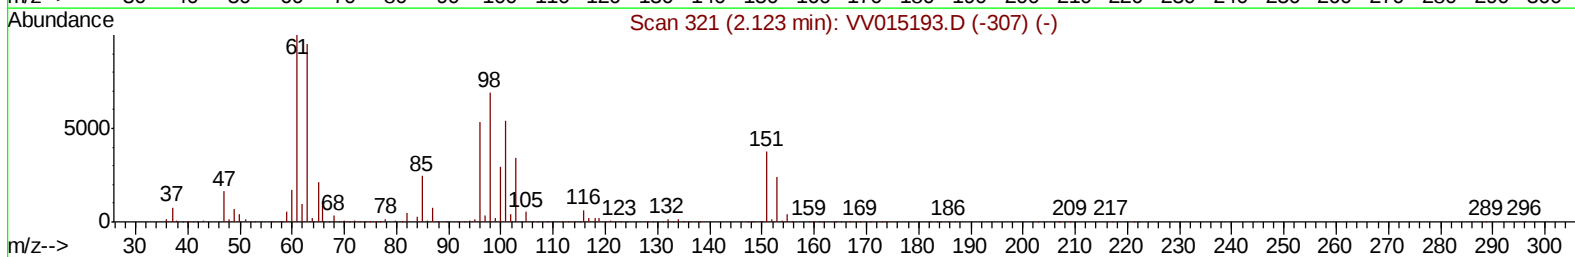
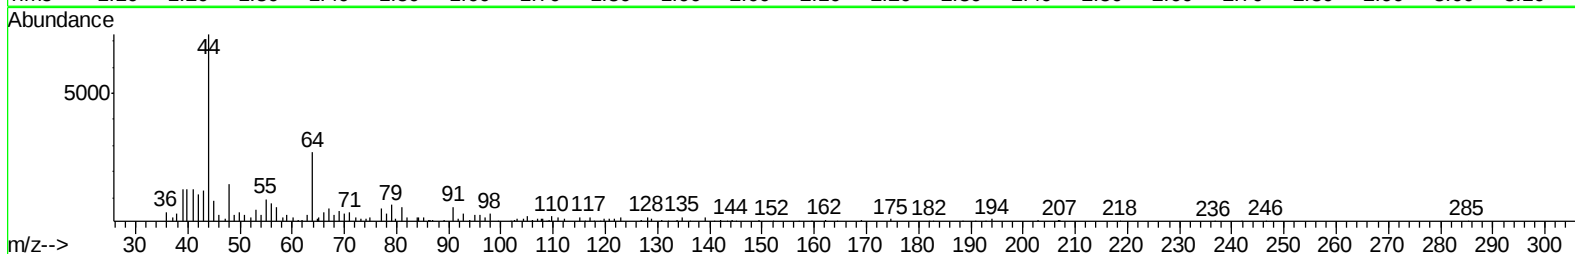


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015207.D
 Acq On : 27 Mar 2020 12:36
 Operator : SY/MD
 Sample : VIBLK75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 01:39:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 01:31:46 2020
 Response via : Initial Calibration

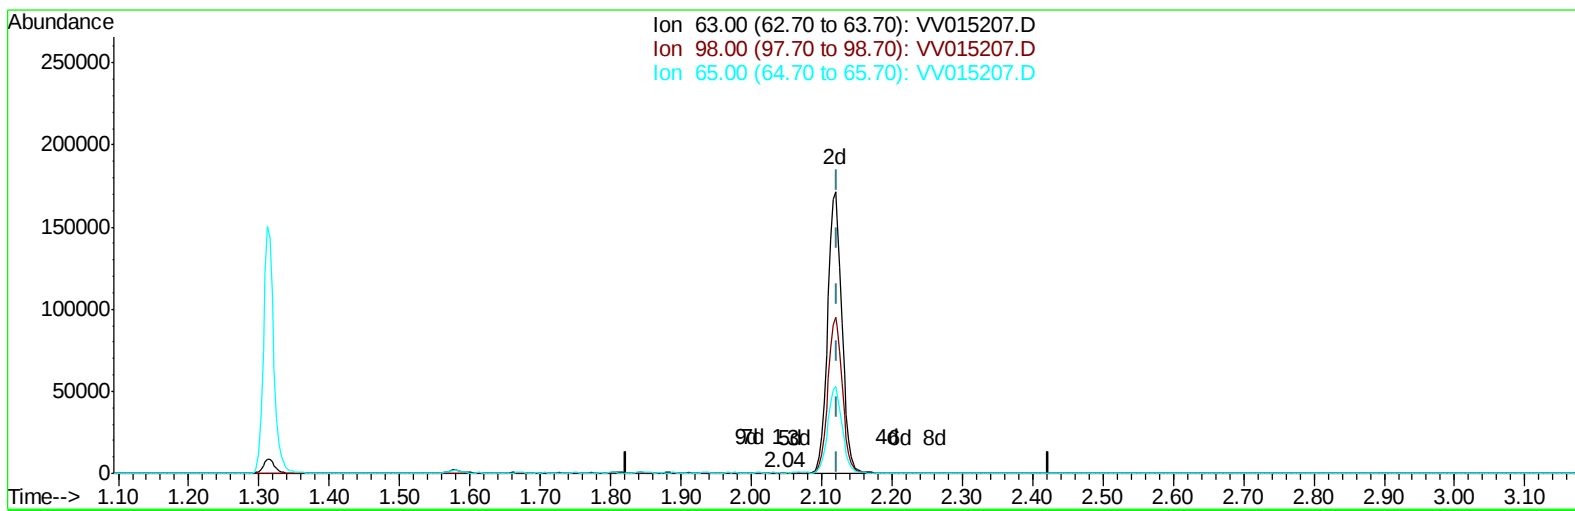

TIC: VV015207.D

(11) 1,1-Dichloroethene-d2 (S)

2.039min (-0.084) 0.05ug/L

response 437

Ion	Exp%	Act%
63.00	100	100
98.00	75.60	66.59
65.00	20.40	24.49
0.00	0.00	0.00