
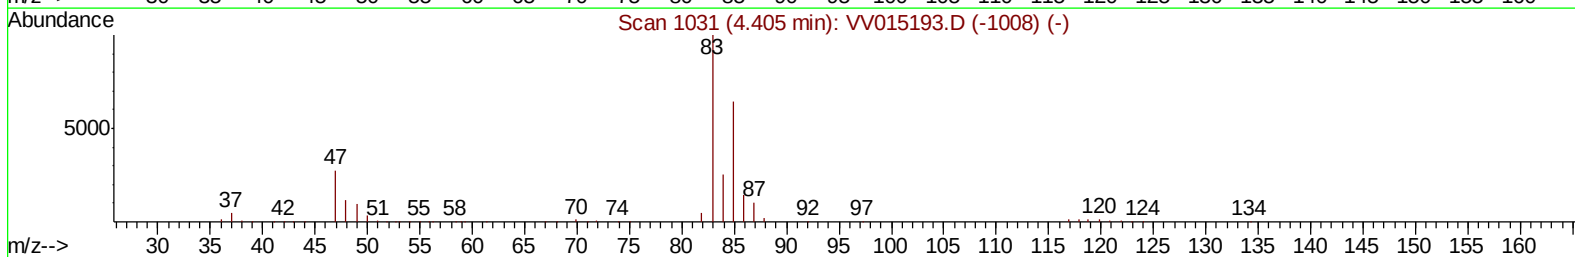
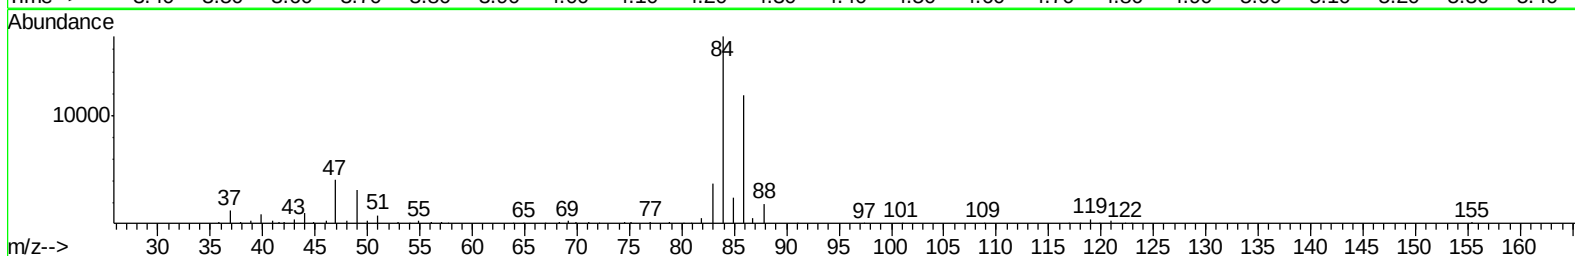


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015207.D
Acq On : 27 Mar 2020 12:36
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 01:39:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 28 01:31:46 2020
Response via : Initial Calibration

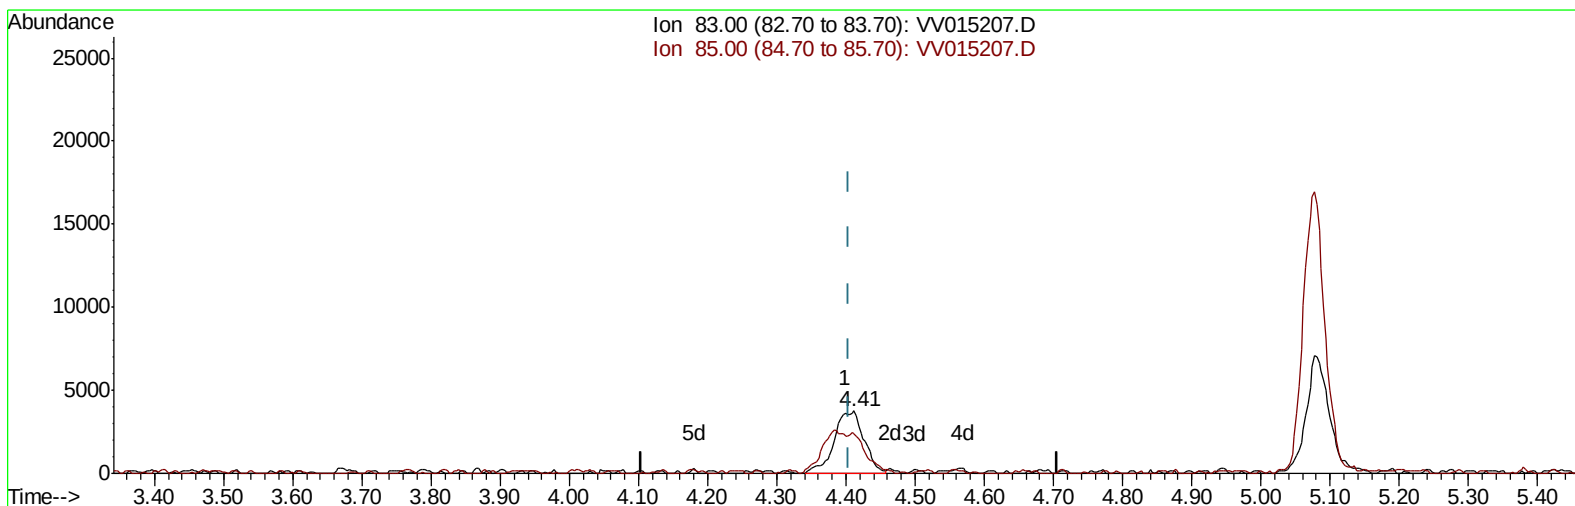

TIC: VV015207.D

(25) Chloroform (T)

4.412min (+0.006) 1.22ug/L m

response 11222

Ion	Exp%	Act%
83.00	100	100
85.00	66.00	63.53
0.00	0.00	0.00
0.00	0.00	0.00