

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015179.D
 Acq On : 26 Mar 2020 20:59
 Operator : SY/MD
 Sample : L1941-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL8

Manual Integrations
 APPROVED

apatel
 3/27/2020 4:17:52 PM

Quant Time: Mar 27 03:39:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 27 03:08:32 2020
 Response via : Initial Calibration

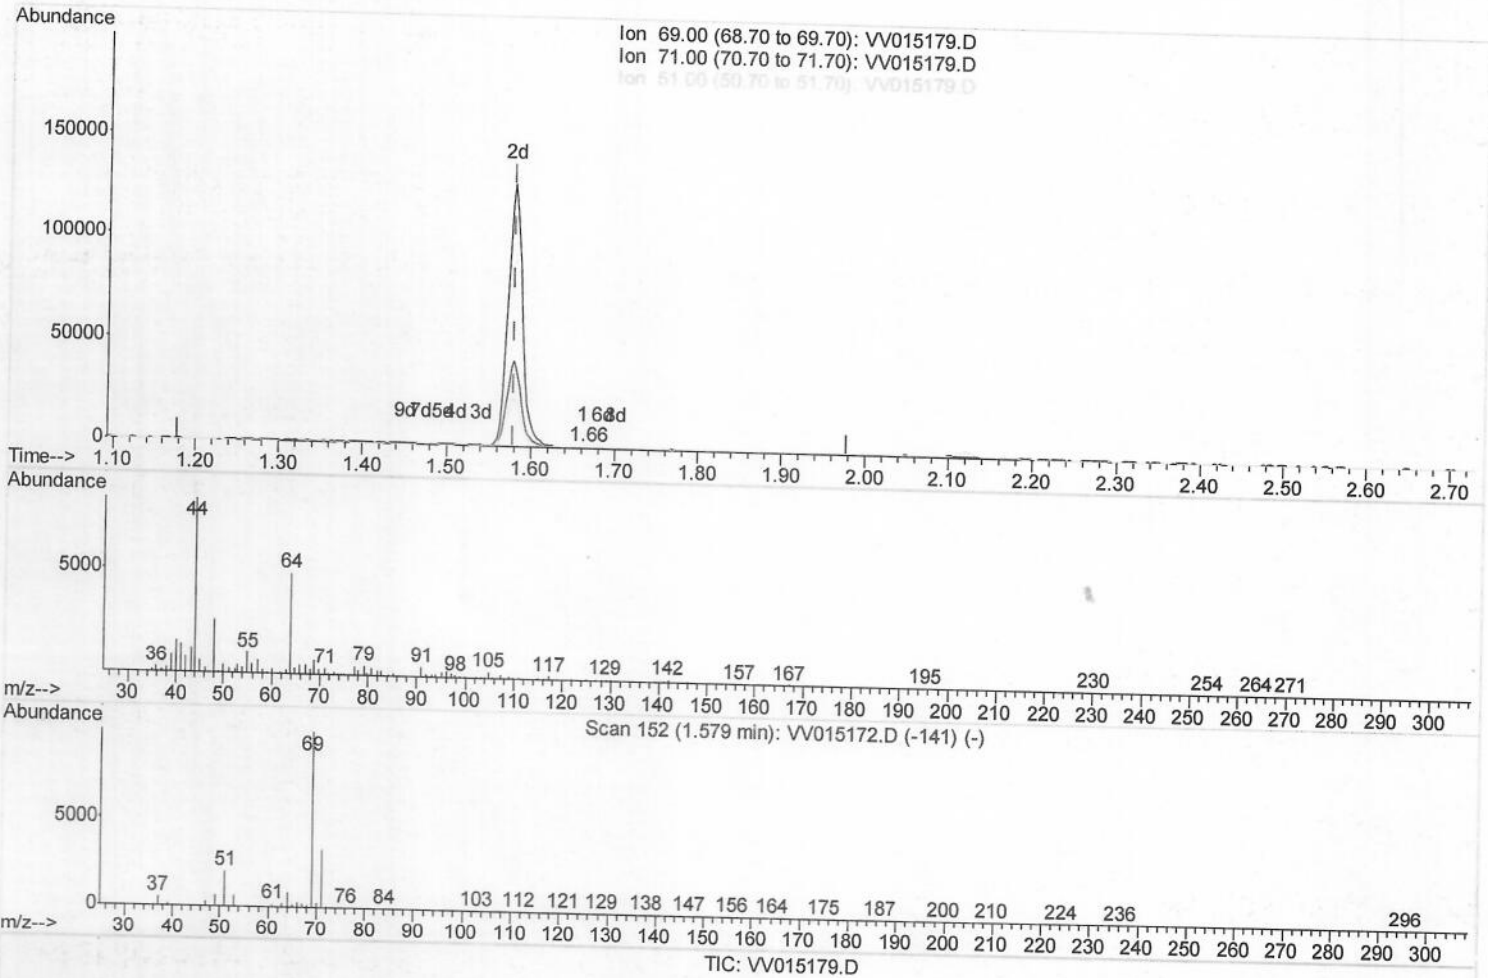

(7) Chloroethane-d5 (S)

1.663min (+0.083) 0.04ug/L

response 142

Ion	Exp%	Act%
69.00	100	100
71.00	31.40	40.14
51.00	28.10	23.94
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015179.D
 Acq On : 26 Mar 2020 20:59
 Operator : SY/MD
 Sample : L1941-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL8

Manual Integrations
 APPROVED

apatel
 3/27/2020 4:17:52 PM

Quant Time: Mar 27 03:39:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 27 03:08:32 2020
 Response via : Initial Calibration

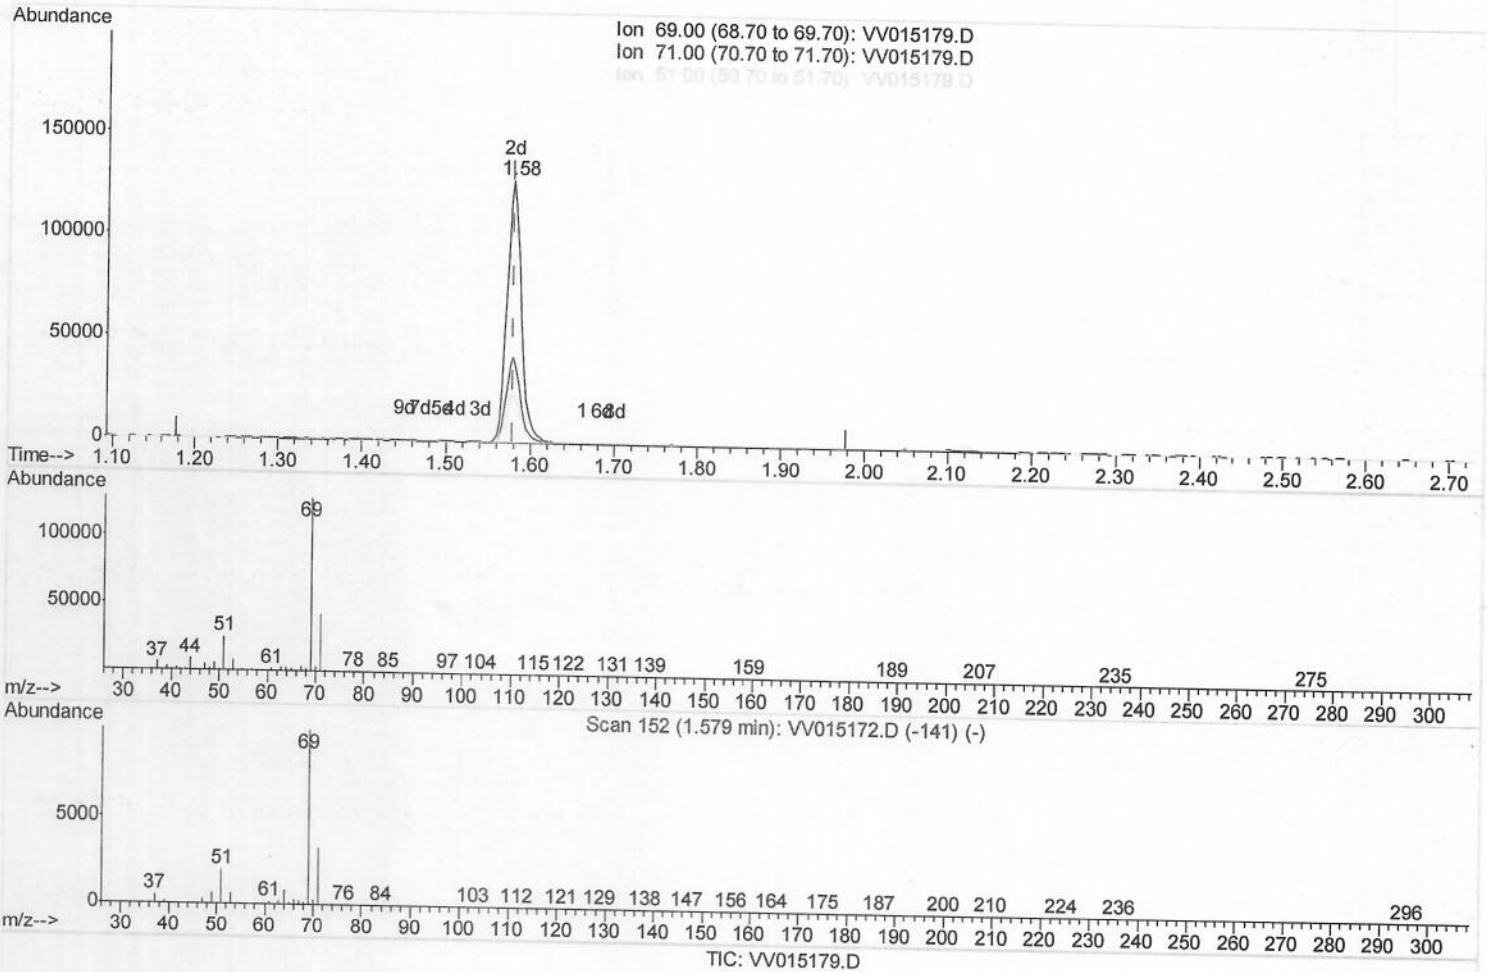

(7) Chloroethane-d5 (S)

1.579min (-0.000) 43.40ug/L m

response 152240

Ion	Exp%	Act%
69.00	100	100
71.00	31.40	0.04#
51.00	28.10	0.02#
0.00	0.00	0.00

MD
 03/30/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015179.D
 Acq On : 26 Mar 2020 20:59
 Operator : SY/MD
 Sample : L1941-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 C0DL8

Manual Integrations
 APPROVED

apatel
 3/27/2020 4:17:52 PM

Quant Time: Mar 27 05:09:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 27 03:08:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.64	114	648577	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	629961	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	277091	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	157008	45.12	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.24%		
7) Chloroethane-d5	1.58	69	152240m	43.40	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.80%		
11) 1,1-Dichloroethene-d2	2.12	63	255490	32.20	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	64.40%		
21) 2-Butanone-d5	3.94	46	234690	67.74	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	67.74%		
24) Chloroform-d	4.38	84	289817	38.00	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	76.00%		
26) 1,2-Dichloroethane-d4	5.06	65	196898	39.11	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.22%		
32) Benzene-d6	5.08	84	567201	43.77	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.54%		
36) 1,2-Dichloropropane-d6	6.10	67	191914	41.06	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	82.12%		
41) Toluene-d8	7.34	98	530327	45.16	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.32%		
43) trans-1,3-Dichloropropene-	7.64	79	97499	38.30	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	76.60%		
47) 2-Hexanone-d5	8.12	63	189642	69.39	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	69.39%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	277899	35.01	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	70.02%		
64) 1,2-Dichlorobenzene-d4	11.65	152	204774	39.58	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.16%#		
Target Compounds						
25) Chloroform	4.41	83	9366	1.083	ug/L	98
33) Benzene	5.13	78	62542	3.335	ug/L	100
51) Chlorobenzene	8.90	112	248331	18.581	ug/L	98
62) 1,3-Dichlorobenzene	11.21	146	35933	3.868	ug/L	94
63) 1,4-Dichlorobenzene	11.30	146	186459	19.867	ug/L	97
65) 1,2-Dichlorobenzene	11.67	146	191347	20.314	ug/L	95
68) 1,2,4-trichlorobenzene	13.29	180	133756	23.588	ug/L	99
70) 1,2,3-Trichlorobenzene	13.77	180	44971	7.920	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
 03/30/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015179.D
 Acq On : 26 Mar 2020 20:59
 Operator : SY/MD
 Sample : L1941-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 C0DL8

Manual Integrations
 APPROVED

apatel
 3/27/2020 4:17:52 PM

Quant Time: Mar 27 05:09:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 27 03:08:32 2020
 Response via : Initial Calibration

