

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015198.D
 Acq On : 27 Mar 2020 06:35
 Operator : SY/MD
 Sample : L1976-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ5

Manual Integrations
 APPROVED

apatel
 3/27/2020 4:18:27 PM

Quant Time: Mar 27 08:16:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 27 06:56:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	591228	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	559085	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	236312	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	147269	46.43	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.86%
7) Chloroethane-d5	1.58	69	154419	48.29	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.58%
11) 1,1-Dichloroethene-d2	2.12	63	233097	32.23	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.46%
21) 2-Butanone-d5	3.93	46	278033	88.03	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.03%
24) Chloroform-d	4.38	84	320385	46.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.16%
26) 1,2-Dichloroethane-d4	5.06	65	221246	48.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.42%
32) Benzene-d6	5.08	84	620772	53.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.96%
36) 1,2-Dichloropropane-d6	6.10	67	208203	50.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.38%
41) Toluene-d8	7.34	98	569969	54.69	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.38%
43) trans-1,3-Dichloropropene-	7.64	79	72483	32.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.16%
47) 2-Hexanone-d5	8.12	63	212115	87.45	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.45%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	320624	45.51	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.02%
64) 1,2-Dichlorobenzene-d4	11.65	152	216360	49.04	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.08%

Target Compounds

					Ovalue
5) Vinyl chloride	1.32	62	21024	3.623 ug/L	# 76
20) cis-1,2-Dichloroethene	3.94	96	160022	34.665 ug/L	98
25) Chloroform	4.40	83	7960m	1.009 ug/L	
34) Trichloroethene	5.94	95	130628	30.127 ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015198.D
Acq On : 27 Mar 2020 06:35
Operator : SY/MD
Sample : L1976-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
ETTJ5

Manual Integrations
APPROVED

apatel
3/27/2020 4:18:27 PM

Quant Time: Mar 27 08:16:18 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 27 06:56:02 2020
Response via : Initial Calibration

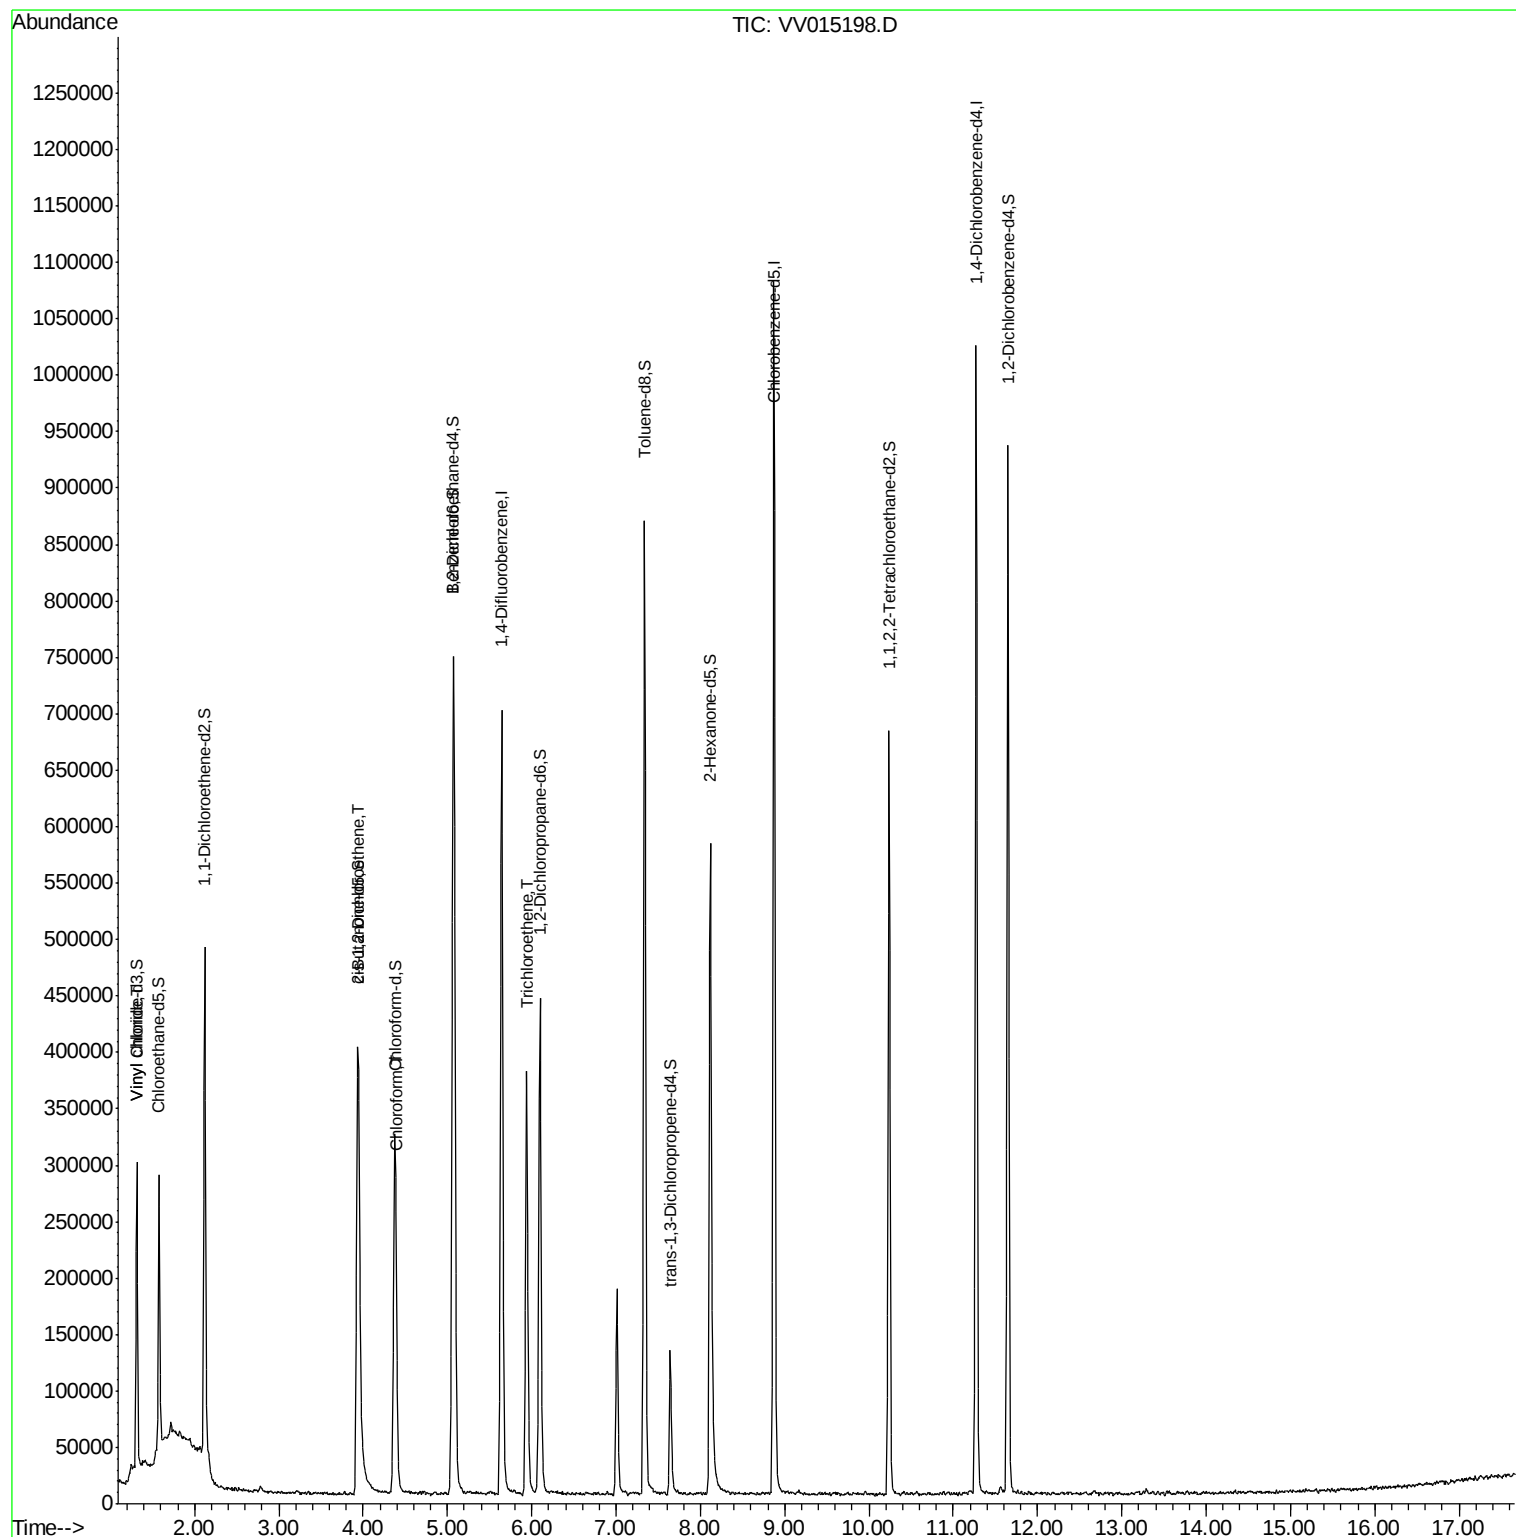

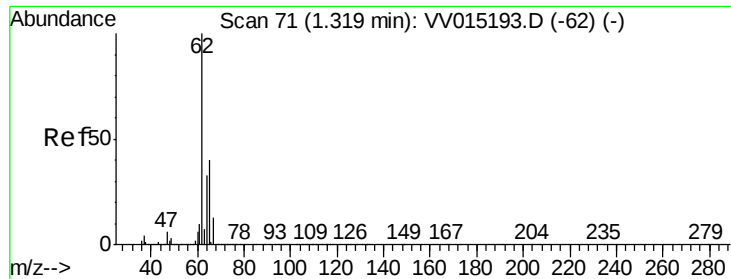

#5

Vinyl chloride

Concen: 3.623 ug/L

RT: 1.32 min Scan# 71

Delta R.T. -0.00 min

Lab File: VV015198.D

Acq: 27 Mar 2020 06:35

Instrument :

MSVOA_V





ClientSampled :

ETTJ5

Tot Ion	Ratio	Lower	Upper
62	100		
64	45.8	22.8	42.4#

Manual Integrations
APPROVED

apatel
3/27/2020 4:18:27 PM

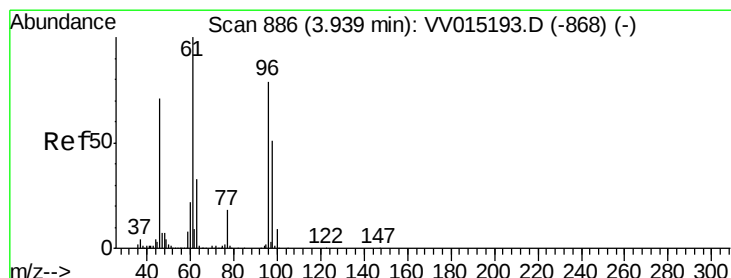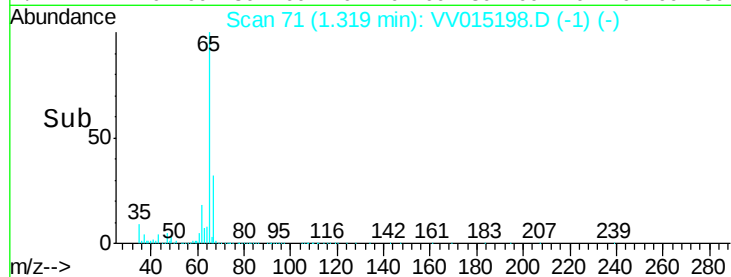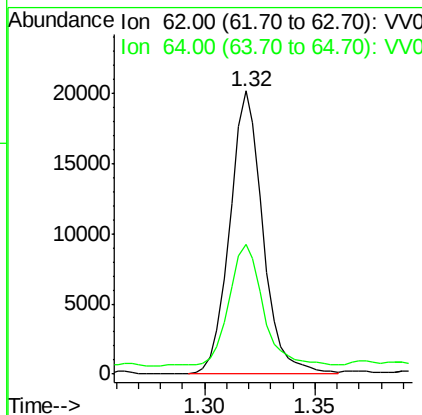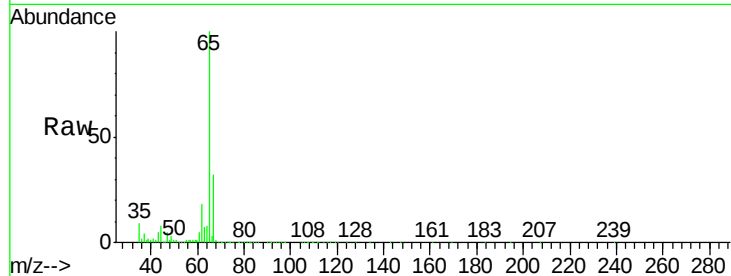

#20

cis-1,2-Dichloroethene

Concen: 34.665 ug/L




RT: 3.94 min Scan# 886


Delta R.T. -0.00 min

Lab File: VV015198.D

Acq: 27 Mar 2020 06:35

Tgt Ion	Ratio	Lower	Upper
96	100		
61	127.0	90.2	167.4
68	0.2	0.1	0.3

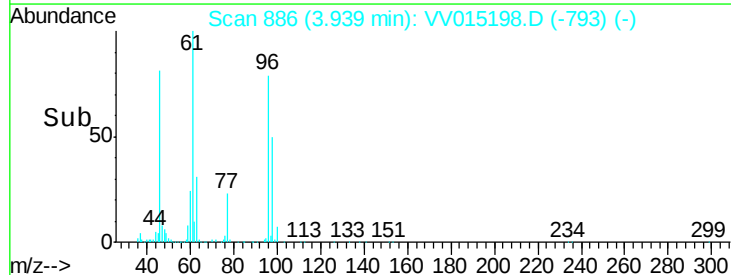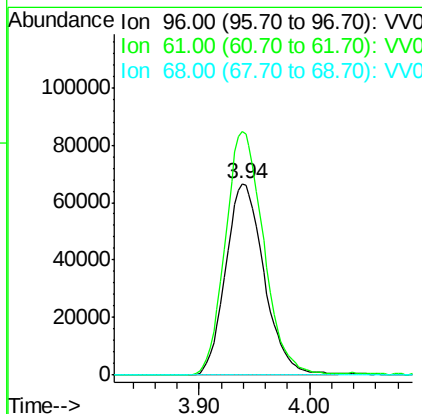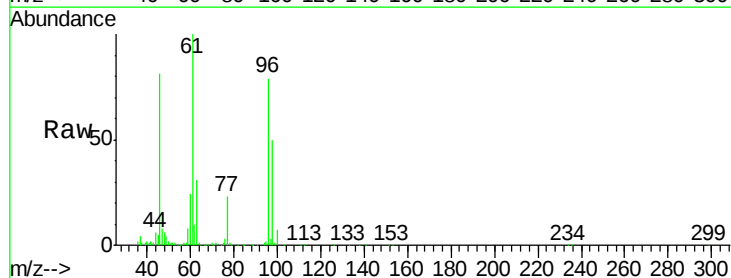

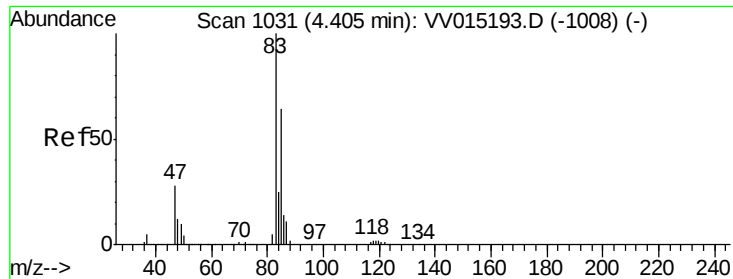





#25
Chloroform
Concen: 1.009 ug/L m
RT: 4.40 min Scan# 1029
Delta R.T. -0.01 min
Lab File: VV015198.D
Acq: 27 Mar 2020 06:35

Instrument :
MSVOA_V
ClientSampled :
ETTJ5

Tot Ion: 83 Resp: 7960
Ion Ratio Lower Upper
83 100
85 90.2 46.2 85.8#

Manual Integrations
APPROVED

apatel
3/27/2020 4:18:27 PM

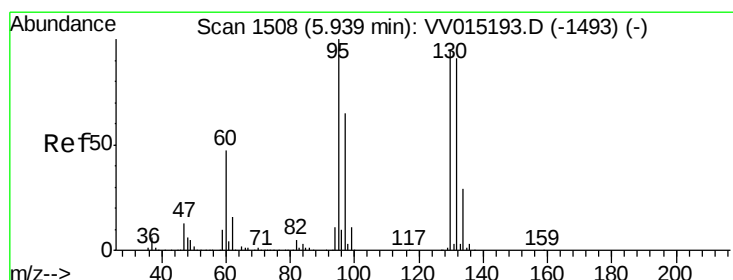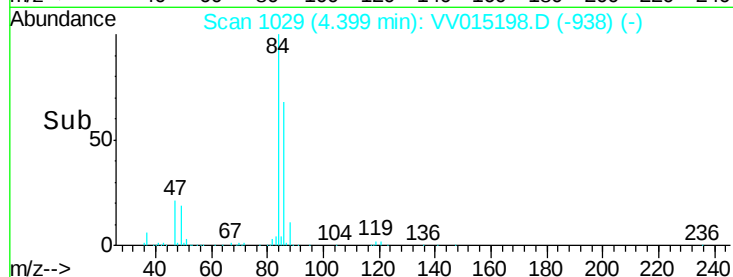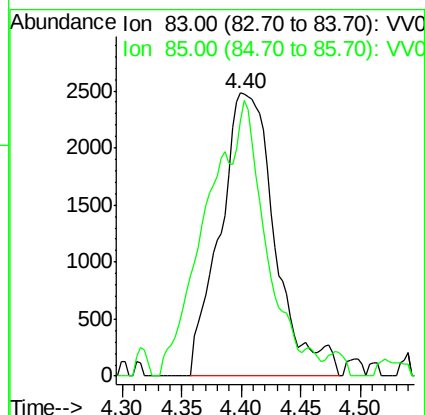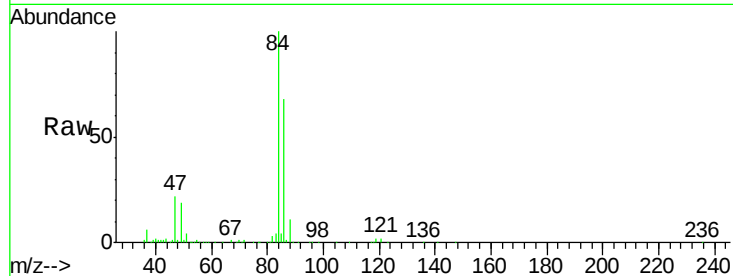

#34
Trichloroethene
Concen: 30.127 ug/L
RT: 5.94 min Scan# 1508
Delta R.T. -0.00 min
Lab File: VV015198.D
Acq: 27 Mar 2020 06:35

Tgt Ion: 95 Resp: 130628
Ion Ratio Lower Upper
95 100
97 61.1 44.8 83.2
132 89.7 63.2 117.4
130 95.6 66.8 124.0

