

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015202.D
 Acq On : 27 Mar 2020 10:34
 Operator : SY/MD
 Sample : L1976-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ1

Quant Time: Mar 28 02:53:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 28 01:31:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	529386	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	499159	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	211724	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	146593	51.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	103.22%
7) Chloroethane-d5	1.58	69	135119	47.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.38%
11) 1,1-Dichloroethene-d2	2.12	63	214859	33.17	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.34%
21) 2-Butanone-d5	3.94	46	208967	73.89	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	73.89%
24) Chloroform-d	4.38	84	271736	43.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.30%
26) 1,2-Dichloroethane-d4	5.06	65	178829	43.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.04%
32) Benzene-d6	5.08	84	513917	50.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.10%
36) 1,2-Dichloropropane-d6	6.10	67	169908	45.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.76%
41) Toluene-d8	7.34	98	465513	50.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.06%
43) trans-1,3-Dichloropropene-	7.64	79	87706	43.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.96%
47) 2-Hexanone-d5	8.12	63	163138	75.33	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.33%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	248959	39.58	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.16%
64) 1,2-Dichlorobenzene-d4	11.65	152	177975	45.02	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.04%

Target Compounds


					Ovalue
5) Vinyl chloride	1.32	62	302779	58.269	ug/L 100
17) trans-1,2-Dichloroethene	2.78	96	6037	1.627	ug/L 92
20) cis-1,2-Dichloroethene	3.94	96	113220	27.392	ug/L # 97
25) Chloroform	4.41	83	6855	0.971	ug/L 82
34) Trichloroethene	5.94	95	11448	2.957	ug/L 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015202.D
Acq On : 27 Mar 2020 10:34
Operator : SY/MD
Sample : L1976-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ1

Quant Time: Mar 28 02:53:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 28 01:31:46 2020
Response via : Initial Calibration

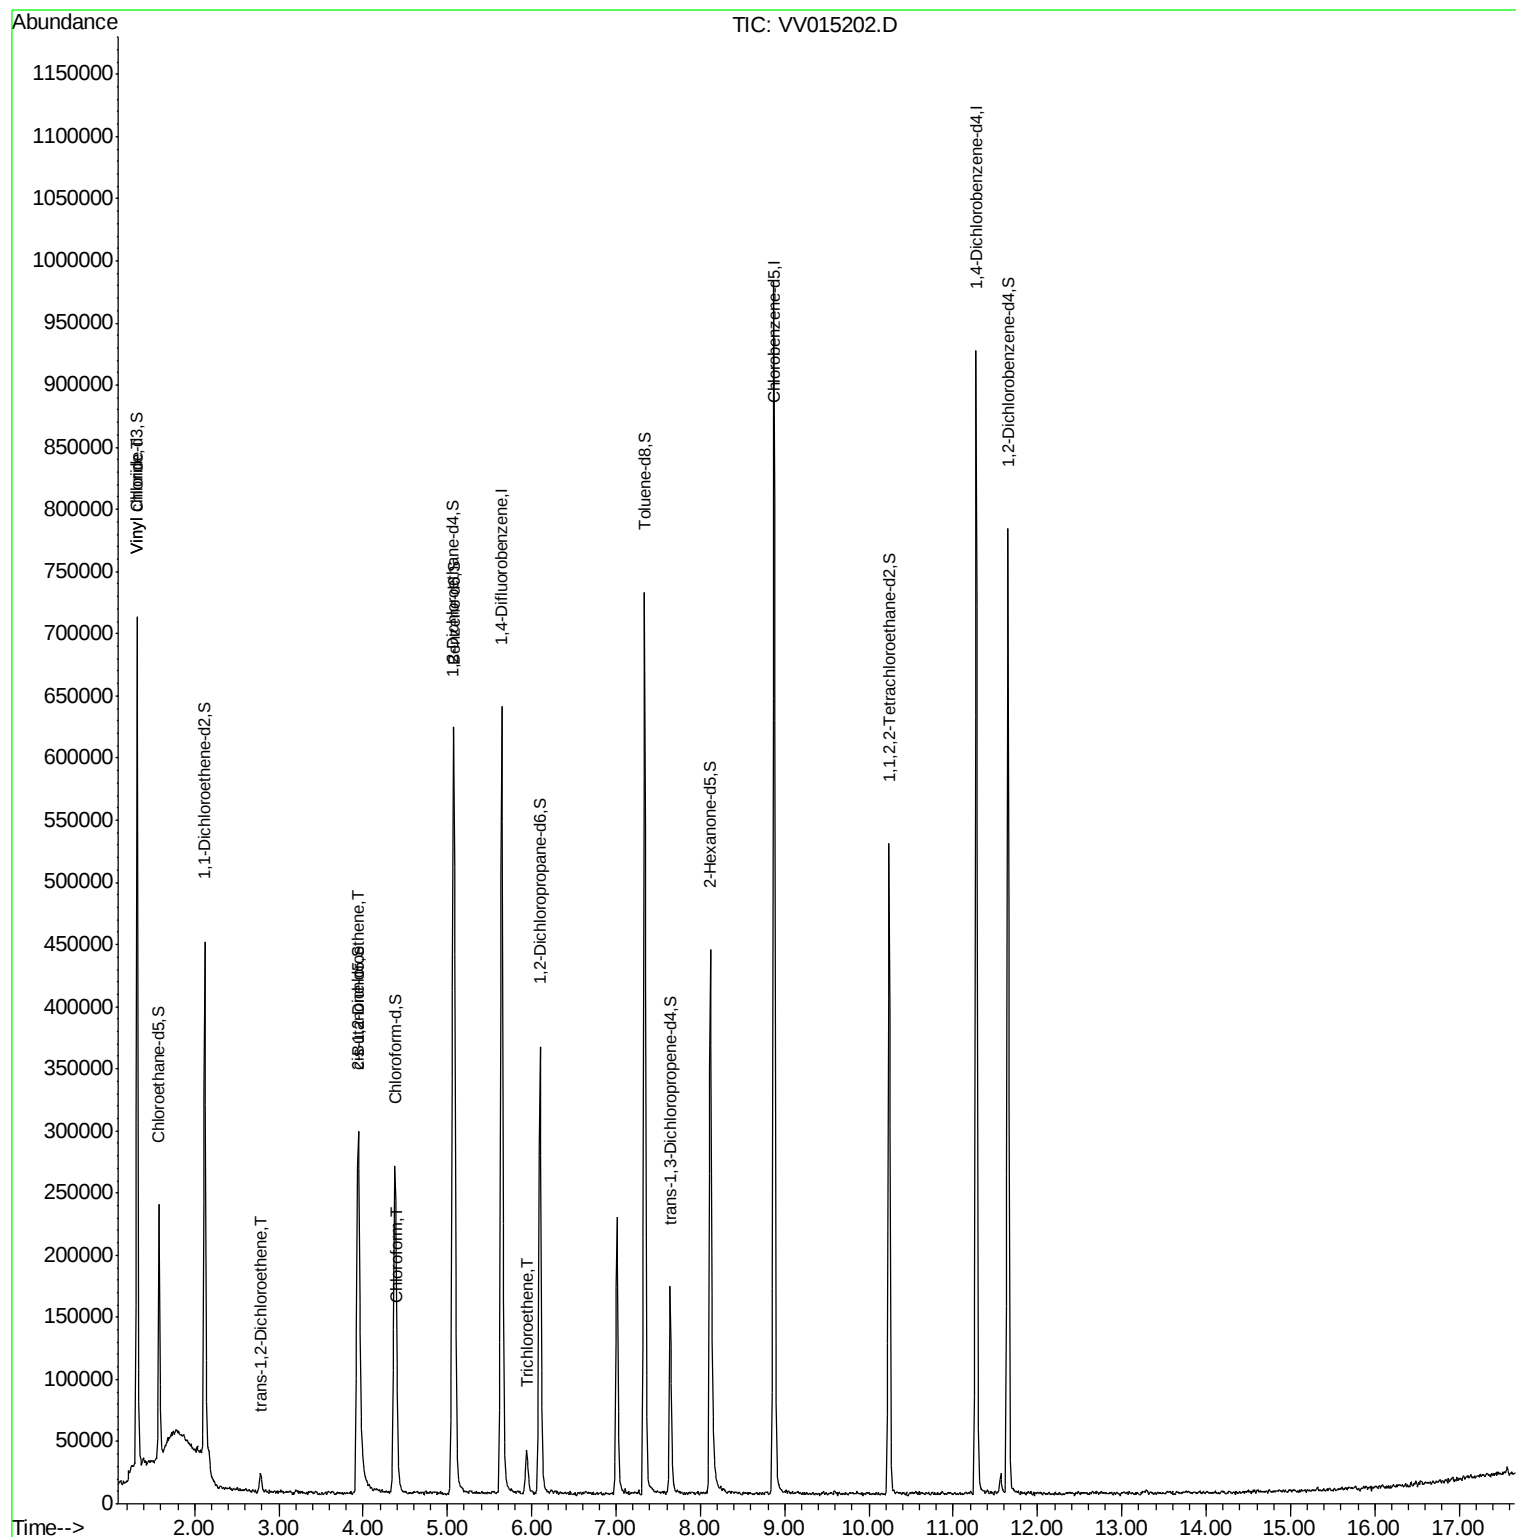

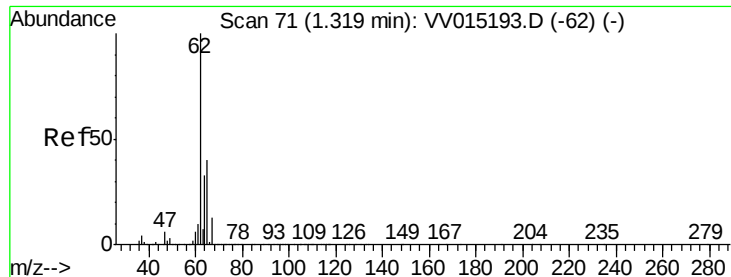

#5

Vinyl chloride

Concen: 58.269 ug/L

RT: 1.32 min Scan# 71

Delta R.T. -0.00 min

Lab File: VV015202.D

Acq: 27 Mar 2020 10:34

Instrument :

MSVOA_V

ClientSampleId :


ETTJ1

Tot Ion: 62 Resp: 302779

Ion Ratio Lower Upper




62 100

64 32.3 22.8 42.4

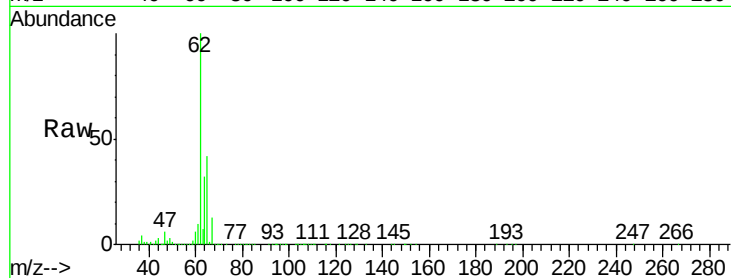

Abundance Ion 62.00 (61.70 to 62.70): VV0

Ion 64.00 (63.70 to 64.70): VV0

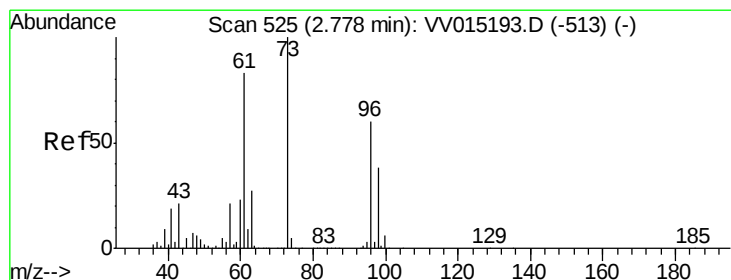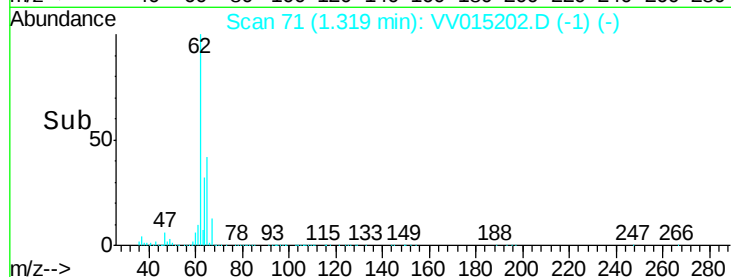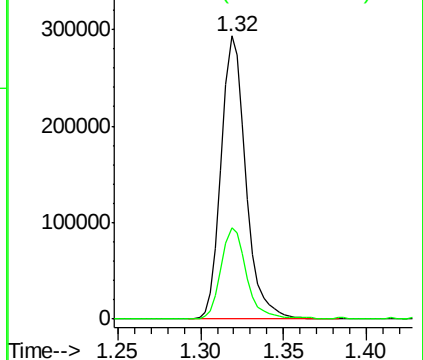

#17

trans-1,2-Dichloroethene

Concen: 1.627 ug/L

RT: 2.78 min Scan# 526

Delta R.T. 0.00 min

Lab File: VV015202.D

Acq: 27 Mar 2020 10:34


Tgt Ion: 96 Resp: 6037

Ion Ratio Lower Upper

96 100

61 124.9 96.4 179.0



98 62.0 43.8 81.4

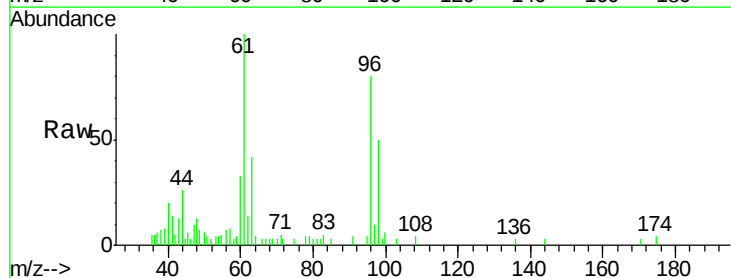


Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.00 (60.70 to 61.70): VV0

Ion 98.00 (97.70 to 98.70): VV0



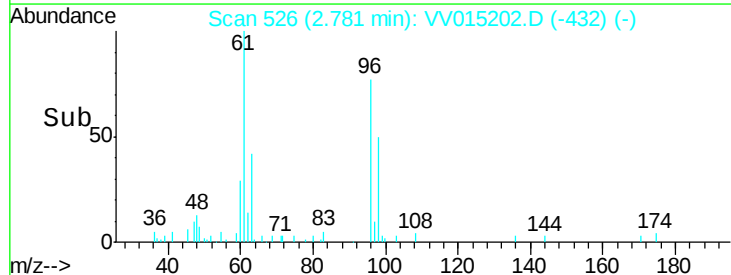
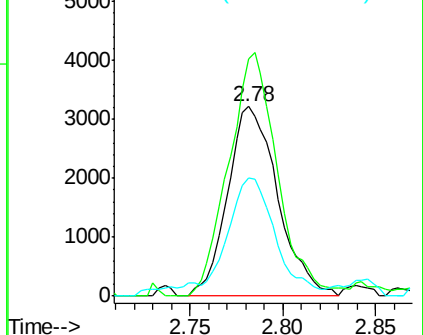


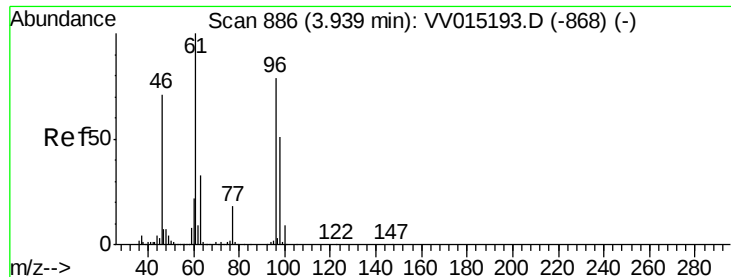

#20
 cis-1,2-Dichloroethene
 Concen: 27.392 ug/L
 RT: 3.94 min Scan# 887
 Delta R.T. 0.00 min
 Lab File: VV015202.D
 Acq: 27 Mar 2020 10:34




Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ1


Tot Ion: 96 Resp: 113220
 Ion Ratio Lower Upper
 96 100
 61 125.4 90.2 167.4
 68 0.0 0.1 0.3#

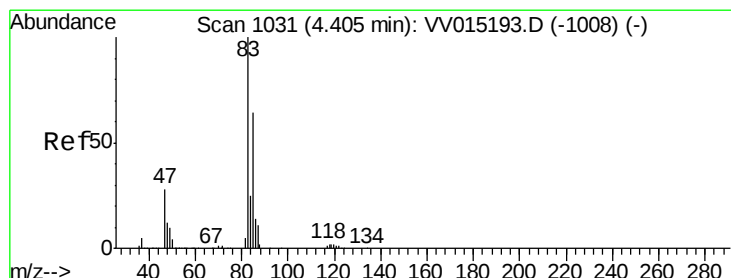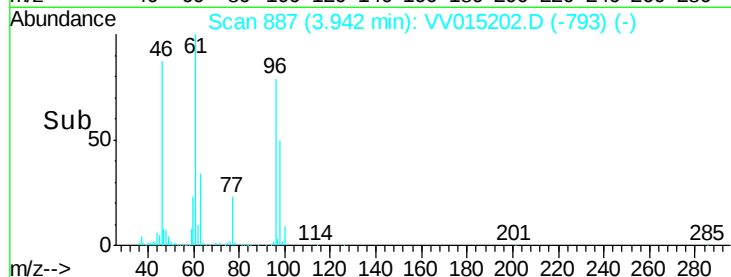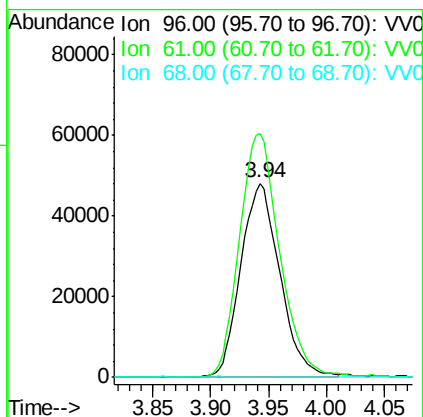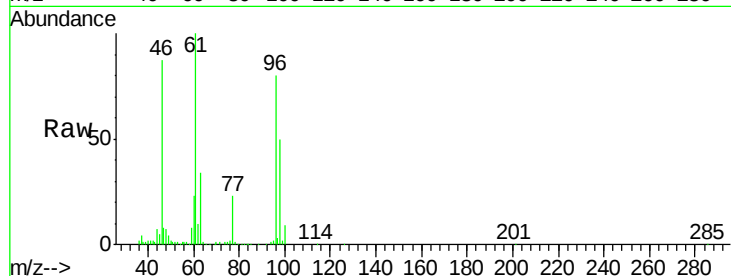

#25
 Chloroform
 Concen: 0.971 ug/L
 RT: 4.41 min Scan# 1033
 Delta R.T. 0.01 min
 Lab File: VV015202.D
 Acq: 27 Mar 2020 10:34

Tgt Ion: 83 Resp: 6855
 Ion Ratio Lower Upper
 83 100
 85 51.8 46.2 85.8

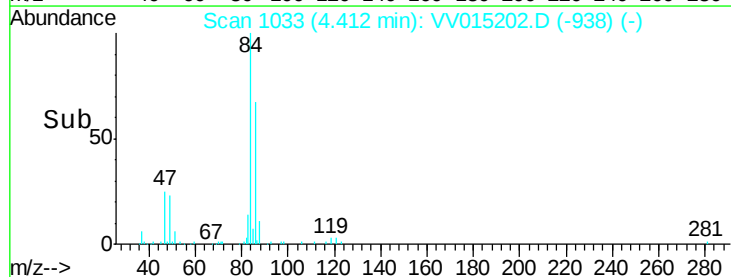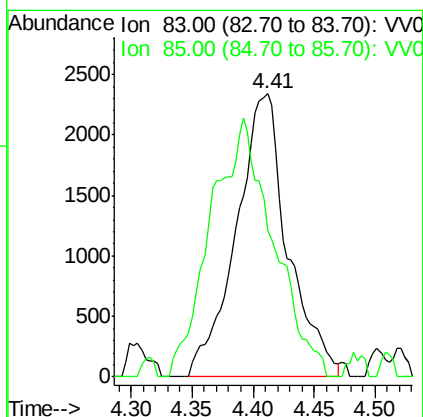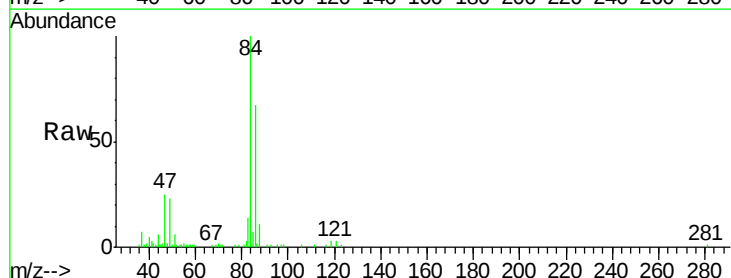

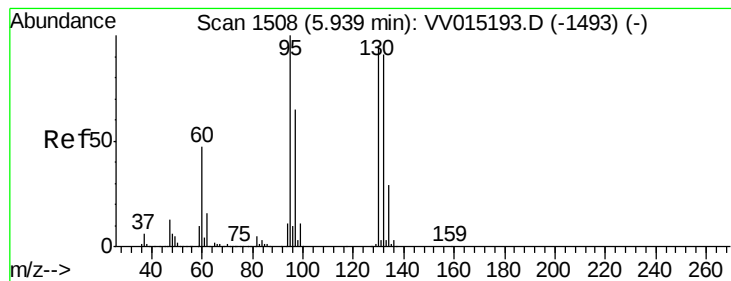

#34

Trichloroethene

Concen: 2.957 ug/L


RT: 5.94 min Scan# 1509

Delta R.T. 0.00 min

Lab File: VV015202.D

Acq: 27 Mar 2020 10:34

Instrument :
MSVOA_V
ClientSampleId :
ETTJ1

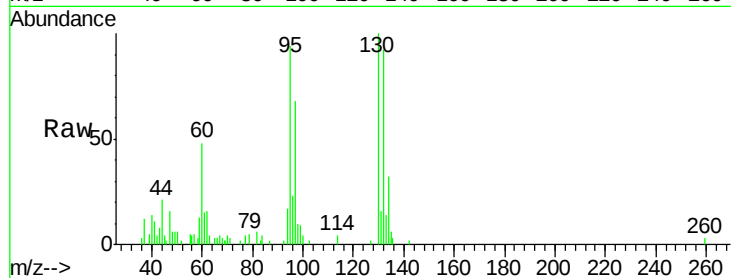

Tot Ion:	95	Resp:	11448
Ion	Ratio	Lower	Upper
95	100		
97	72.7	44.8	83.2
132	98.1	63.2	117.4
130	106.4	66.8	124.0

