

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015173.D
 Acq On : 26 Mar 2020 18:34
 Operator : SY/MD
 Sample : VV0326WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	81	rVB	271619	273956	13.49%	1.506%
2	1.579	146	152	165	rVB	258718	306285	15.08%	1.684%
3	2.119	314	320	333	rVB	455262	639760	31.51%	3.517%
4	3.550	763	765	766	rBV2	1859	796	0.04%	0.004%
5	3.595	775	779	782	rBV5	1836	1682	0.08%	0.009%
6	3.717	815	817	822	rBV6	2442	2276	0.11%	0.013%
7	3.849	851	858	860	rBV7	2287	2353	0.12%	0.013%
8	3.939	873	886	943	rBV	140534	678589	33.42%	3.730%
9	4.376	1006	1022	1044	rBV	358580	892156	43.94%	4.904%
10	4.730	1131	1132	1135	rBV3	1361	851	0.04%	0.005%
11	4.920	1187	1191	1193	rBV5	1549	1153	0.06%	0.006%
12	4.994	1211	1214	1216	rBV4	1102	786	0.04%	0.004%
13	5.074	1221	1239	1264	rBV2	798327	2030522	100.00%	11.161%
14	5.299	1305	1309	1311	rBV5	1796	1429	0.07%	0.008%
15	5.454	1354	1357	1360	rBV4	1416	1027	0.05%	0.006%
16	5.640	1402	1415	1438	rBV	762771	1535379	75.61%	8.440%
17	5.872	1483	1487	1488	rBV4	2019	1398	0.07%	0.008%
18	6.097	1543	1557	1584	rBV2	486672	997838	49.14%	5.485%
19	6.482	1675	1677	1680	rBV4	1529	797	0.04%	0.004%
20	6.579	1703	1707	1711	rVB6	1522	1408	0.07%	0.008%
21	6.630	1721	1723	1725	rBV3	1595	872	0.04%	0.005%
22	6.775	1766	1768	1771	rBV3	1569	936	0.05%	0.005%
23	6.788	1771	1772	1775	rVV3	1135	654	0.03%	0.004%
24	6.849	1789	1791	1796	rBV4	1566	1064	0.05%	0.006%
25	6.875	1796	1799	1802	rVB4	2618	1762	0.09%	0.010%
26	6.913	1807	1811	1812	rBV4	1541	873	0.04%	0.005%
27	7.007	1830	1840	1864	rBV	303817	533684	26.28%	2.934%
28	7.338	1931	1943	1964	rBV	866575	1511523	74.44%	8.309%
29	7.643	2028	2038	2054	rBV	215567	368102	18.13%	2.023%
30	7.897	2113	2117	2122	rBV8	2523	2328	0.11%	0.013%
31	7.923	2123	2125	2126	rBV2	1674	644	0.03%	0.004%
32	7.997	2144	2148	2150	rBV5	3496	2502	0.12%	0.014%
33	8.042	2160	2162	2163	rBV2	2640	1116	0.05%	0.006%
34	8.116	2174	2185	2214	rBV2	742813	1523961	75.05%	8.377%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015173.D
 Acq On : 26 Mar 2020 18:34
 Operator : SY/MD
 Sample : VV0326WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	8.592	2331	2333	2336	rBV3	1062	779	0.04%	0.004%
36	8.646	2347	2350	2352	rBV4	1630	1221	0.06%	0.007%
37	8.730	2374	2376	2378	rBV3	1639	638	0.03%	0.004%
38	8.875	2409	2421	2450	rBV	1209363	1935706	95.33%	10.640%
39	9.225	2527	2530	2532	rBV4	1885	1105	0.05%	0.006%
40	9.347	2565	2568	2570	rBV4	1963	1100	0.05%	0.006%
41	9.379	2574	2578	2581	rBV5	1891	1514	0.07%	0.008%
42	9.396	2581	2583	2585	rBV3	1802	856	0.04%	0.005%
43	9.498	2611	2615	2617	rBV5	3533	2422	0.12%	0.013%
44	9.547	2628	2630	2632	rBV3	2117	1222	0.06%	0.007%
45	9.691	2673	2675	2679	rVV5	1549	874	0.04%	0.005%
46	9.720	2681	2684	2689	rVB6	2004	1435	0.07%	0.008%
47	9.871	2729	2731	2734	rBV4	1329	924	0.05%	0.005%
48	9.891	2734	2737	2739	rVV4	1906	1148	0.06%	0.006%
49	9.907	2739	2742	2744	rVB4	1747	1006	0.05%	0.006%
50	9.997	2768	2770	2773	rBV4	2178	863	0.04%	0.005%
51	10.035	2780	2782	2785	rBV4	1400	988	0.05%	0.005%
52	10.093	2796	2800	2801	rBV4	1274	868	0.04%	0.005%
53	10.135	2810	2813	2814	rBV3	2195	1545	0.08%	0.008%
54	10.154	2818	2819	2821	rVV2	2139	1081	0.05%	0.006%
55	10.167	2821	2823	2827	rVB5	3174	1866	0.09%	0.010%
56	10.238	2833	2845	2863	rBV	831652	1291839	63.62%	7.101%
57	10.508	2925	2929	2932	rVB6	1887	1289	0.06%	0.007%
58	10.682	2981	2983	2986	rBV4	1969	1080	0.05%	0.006%
59	10.704	2988	2990	2993	rVV3	1451	941	0.05%	0.005%
60	10.801	3014	3020	3023	rBV7	3227	3894	0.19%	0.021%
61	10.977	3073	3075	3080	rVB5	1402	929	0.05%	0.005%
62	10.997	3080	3081	3085	rBV3	1566	785	0.04%	0.004%
63	11.154	3128	3130	3133	rVB3	1607	792	0.04%	0.004%
64	11.177	3133	3137	3138	rBV4	1908	1281	0.06%	0.007%
65	11.270	3154	3166	3184	rBV	1183063	1805988	88.94%	9.927%
66	11.495	3233	3236	3238	rBV3	2372	1440	0.07%	0.008%
67	11.646	3270	3283	3301	rBV	1116253	1733560	85.38%	9.529%
68	11.887	3355	3358	3360	rBV4	1704	1086	0.05%	0.006%
69	11.913	3364	3366	3368	rBV3	1221	644	0.03%	0.004%
70	11.926	3368	3370	3375	rVB6	1575	1036	0.05%	0.006%
71	11.974	3380	3385	3387	rBV6	1271	1218	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015173.D
 Acq On : 26 Mar 2020 18:34
 Operator : SY/MD
 Sample : VV0326WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	12.026	3399	3401	3406	rVB5	1895	1325	0.07%	0.007%
73	12.045	3406	3407	3412	rBV5	1868	1196	0.06%	0.007%
74	12.106	3423	3426	3427	rBV3	2021	1087	0.05%	0.006%
75	12.116	3427	3429	3432	rVB3	3803	1992	0.10%	0.011%
76	12.148	3435	3439	3443	rBV6	2078	2039	0.10%	0.011%
77	12.251	3468	3471	3473	rBV3	1356	880	0.04%	0.005%
78	12.347	3499	3501	3502	rBV2	2058	946	0.05%	0.005%
79	12.444	3527	3531	3535	rBV6	2362	2243	0.11%	0.012%
80	12.566	3566	3569	3571	rBV4	2518	1390	0.07%	0.008%
81	12.672	3593	3602	3614	rVB4	7286	13944	0.69%	0.077%
82	12.720	3614	3617	3618	rBV3	1339	812	0.04%	0.004%
83	12.772	3629	3633	3636	rVV6	1760	1557	0.08%	0.009%
84	12.849	3652	3657	3658	rBV5	1591	1287	0.06%	0.007%
85	13.013	3705	3708	3712	rBV5	2828	2618	0.13%	0.014%
86	13.032	3712	3714	3716	rBV3	1238	706	0.03%	0.004%
87	13.112	3735	3739	3743	rVV7	1669	1610	0.08%	0.009%
88	13.141	3746	3748	3750	rBV3	1382	729	0.04%	0.004%
89	13.177	3756	3759	3764	rVB6	3382	2641	0.13%	0.015%
90	13.257	3782	3784	3785	rBV2	1971	885	0.04%	0.005%
91	13.366	3815	3818	3820	rBV4	2578	1538	0.08%	0.008%
92	13.386	3820	3824	3826	rVV4	1739	1380	0.07%	0.008%
93	13.479	3851	3853	3854	rBV2	1940	766	0.04%	0.004%
94	13.630	3896	3900	3906	rBV9	2077	2957	0.15%	0.016%
95	13.768	3938	3943	3952	rBV9	7586	11304	0.56%	0.062%
96	13.974	4003	4007	4012	rBV7	1762	2013	0.10%	0.011%
97	14.145	4057	4060	4062	rBV3	1697	1219	0.06%	0.007%
98	14.440	4150	4152	4155	rBV4	2163	1132	0.06%	0.006%
99	14.495	4167	4169	4171	rBV3	2027	883	0.04%	0.005%
100	14.585	4194	4197	4200	rBV4	3013	1928	0.09%	0.011%


Sum of corrected areas: 18192432

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015173.D
Acq On : 26 Mar 2020 18:34
Operator : SY/MD
Sample : VV0326WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK93

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

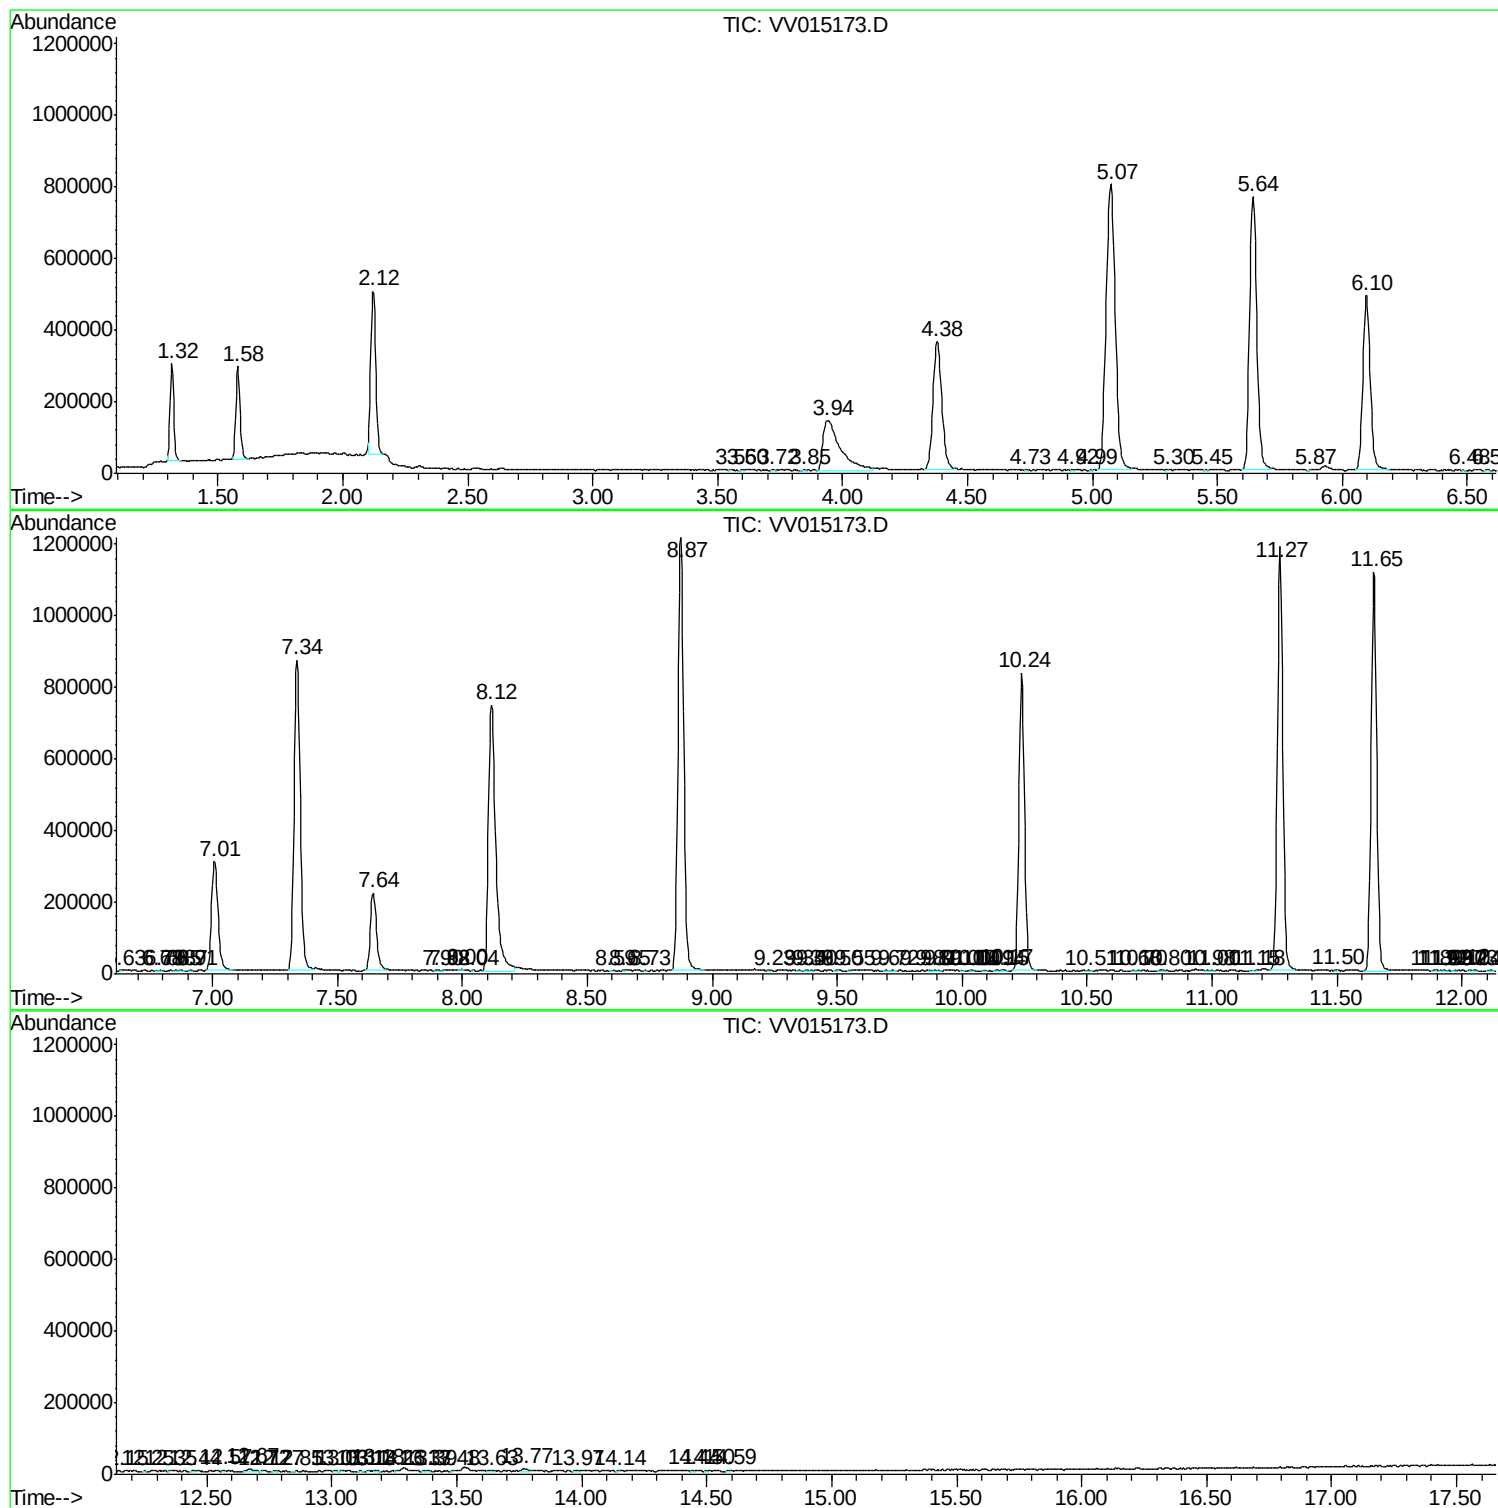

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015173.D
Acq On : 26 Mar 2020 18:34
Operator : SY/MD
Sample : VV0326WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK93

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015173.D
Acq On : 26 Mar 2020 18:34
Operator : SY/MD
Sample : VV0326WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK93

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc