

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015175.D
 Acq On : 26 Mar 2020 19:22
 Operator : SY/MD
 Sample : L2045-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	84	rVB	269739	270913	13.74%	1.733%
2	1.579	147	152	167	rVB	222244	255619	12.96%	1.635%
3	2.119	314	320	349	rVB	484720	767915	38.94%	4.913%
4	3.409	718	721	722	rBV3	1880	1027	0.05%	0.007%
5	3.505	748	751	753	rBV4	2574	1882	0.10%	0.012%
6	3.553	762	766	771	rBV7	2557	2507	0.13%	0.016%
7	3.640	791	793	797	rBV4	1120	682	0.03%	0.004%
8	3.833	851	853	857	rVB4	2045	1194	0.06%	0.008%
9	3.888	868	870	873	rBV4	1854	1204	0.06%	0.008%
10	3.942	875	887	930	rVV	91654	391215	19.84%	2.503%
11	4.380	1009	1023	1048	rVB	282375	691588	35.07%	4.424%
12	4.692	1119	1120	1122	rBV2	1229	491	0.02%	0.003%
13	4.830	1161	1163	1165	rBV3	1724	878	0.04%	0.006%
14	4.852	1165	1170	1172	rBV5	2549	2351	0.12%	0.015%
15	5.074	1223	1239	1262	rBV2	664481	1656210	83.98%	10.595%
16	5.489	1362	1368	1371	rBV7	2910	3333	0.17%	0.021%
17	5.640	1403	1415	1444	rBV	793272	1563839	79.30%	10.004%
18	6.013	1528	1531	1534	rBV4	2591	2058	0.10%	0.013%
19	6.097	1541	1557	1581	rBV	392088	807035	40.92%	5.163%
20	6.206	1589	1591	1594	rBV4	2107	1136	0.06%	0.007%
21	6.473	1672	1674	1677	rVB3	1614	937	0.05%	0.006%
22	6.556	1694	1700	1701	rBV5	2943	2190	0.11%	0.014%
23	6.595	1710	1712	1713	rBV3	1649	739	0.04%	0.005%
24	6.637	1722	1725	1728	rBV4	2005	1756	0.09%	0.011%
25	6.714	1744	1749	1754	rBV8	1745	2252	0.11%	0.014%
26	6.785	1769	1771	1773	rBV3	1639	869	0.04%	0.006%
27	6.804	1773	1777	1780	rVV5	1620	1484	0.08%	0.009%
28	6.859	1790	1794	1795	rBV4	1932	1435	0.07%	0.009%
29	6.878	1798	1800	1803	rVB4	1780	1029	0.05%	0.007%
30	6.907	1803	1809	1812	rBV7	1888	2025	0.10%	0.013%
31	7.010	1825	1841	1857	rBV	240339	437398	22.18%	2.798%
32	7.257	1911	1918	1922	rBV9	2696	3513	0.18%	0.022%
33	7.338	1931	1943	1962	rBV	785425	1358327	68.88%	8.690%
34	7.643	2027	2038	2060	rBV	171491	300028	15.21%	1.919%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015175.D
 Acq On : 26 Mar 2020 19:22
 Operator : SY/MD
 Sample : L2045-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	8.058	2165	2167	2171	rBV6	1390	729	0.04%	0.005%
36	8.116	2172	2185	2214	rBV2	492855	1003438	50.88%	6.419%
37	8.460	2289	2292	2298	rBV7	2168	2284	0.12%	0.015%
38	8.569	2324	2326	2328	rBV3	1691	1051	0.05%	0.007%
39	8.627	2340	2344	2345	rBV4	1649	1165	0.06%	0.007%
40	8.756	2381	2384	2386	rBV3	1214	934	0.05%	0.006%
41	8.875	2409	2421	2440	rBV	1225136	1972056	100.00%	12.616%
42	9.351	2566	2569	2571	rBV4	2229	1490	0.08%	0.010%
43	9.389	2579	2581	2586	rBV6	1527	1480	0.08%	0.009%
44	9.486	2609	2611	2613	rBV3	1532	982	0.05%	0.006%
45	9.540	2623	2628	2632	rBV7	2539	2996	0.15%	0.019%
46	9.691	2673	2675	2678	rBV3	1157	602	0.03%	0.004%
47	9.707	2678	2680	2683	rVB3	1530	552	0.03%	0.004%
48	9.730	2683	2687	2690	rBV6	2249	1722	0.09%	0.011%
49	9.768	2697	2699	2701	rBV2	2286	804	0.04%	0.005%
50	9.881	2732	2734	2735	rBV2	1227	475	0.02%	0.003%
51	9.916	2742	2745	2747	rBV4	1724	979	0.05%	0.006%
52	9.945	2747	2754	2756	rBV6	2924	3420	0.17%	0.022%
53	10.010	2771	2774	2776	rBV4	2631	1465	0.07%	0.009%
54	10.145	2814	2816	2820	rBV5	1727	1144	0.06%	0.007%
55	10.238	2834	2845	2862	rBV	569786	893043	45.28%	5.713%
56	10.334	2872	2875	2878	rBV4	2010	1584	0.08%	0.010%
57	10.662	2975	2977	2980	rBV3	1059	703	0.04%	0.004%
58	10.714	2990	2993	2994	rBV3	2612	1485	0.08%	0.009%
59	10.746	2999	3003	3004	rBV3	1448	1015	0.05%	0.006%
60	10.791	3015	3017	3018	rBV2	1014	424	0.02%	0.003%
61	10.849	3031	3035	3039	rBV7	2500	2279	0.12%	0.015%
62	10.865	3039	3040	3046	rVB6	2019	1598	0.08%	0.010%
63	10.932	3051	3061	3063	rBV10	3619	4437	0.22%	0.028%
64	10.987	3074	3078	3080	rBV5	1335	1201	0.06%	0.008%
65	11.080	3103	3107	3108	rBV4	1521	982	0.05%	0.006%
66	11.125	3119	3121	3125	rVB4	2418	1488	0.08%	0.010%
67	11.151	3125	3129	3131	rBV4	2568	1998	0.10%	0.013%
68	11.270	3155	3166	3189	rVB	1189104	1826624	92.63%	11.685%
69	11.563	3250	3257	3266	rBV10	7902	12840	0.65%	0.082%
70	11.646	3272	3283	3302	rBV	829842	1306807	66.27%	8.360%
71	11.723	3305	3307	3308	rBV2	1746	517	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015175.D
 Acq On : 26 Mar 2020 19:22
 Operator : SY/MD
 Sample : L2045-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.923	3363	3369	3372	rBV7	2535	2718	0.14%	0.017%
73	11.977	3384	3386	3388	rVB3	1358	429	0.02%	0.003%
74	11.993	3388	3391	3392	rBV3	1527	896	0.05%	0.006%
75	12.061	3409	3412	3415	rBV5	1972	1477	0.07%	0.009%
76	12.112	3424	3428	3430	rBV5	2129	1465	0.07%	0.009%
77	12.151	3437	3440	3442	rBV4	1428	1100	0.06%	0.007%
78	12.180	3447	3449	3452	rBV4	1008	517	0.03%	0.003%
79	12.219	3456	3461	3462	rBV4	1495	1140	0.06%	0.007%
80	12.366	3505	3507	3510	rBV3	2197	1490	0.08%	0.010%
81	12.505	3548	3550	3553	rVB3	1514	495	0.03%	0.003%
82	12.524	3553	3556	3559	rBV6	1513	910	0.05%	0.006%
83	12.881	3665	3667	3670	rBV4	1420	762	0.04%	0.005%
84	13.038	3713	3716	3717	rBV3	1442	727	0.04%	0.005%
85	13.093	3729	3733	3736	rBV6	892	695	0.04%	0.004%
86	13.148	3748	3750	3759	rVB8	2267	2376	0.12%	0.015%
87	13.193	3761	3764	3766	rBV4	2563	1484	0.08%	0.009%
88	13.717	3925	3927	3930	rVB3	2523	1183	0.06%	0.008%
89	13.733	3930	3932	3934	rBV3	1217	568	0.03%	0.004%
90	13.743	3934	3935	3936	rBV	1202	429	0.02%	0.003%
91	14.045	4027	4029	4036	rVB7	2028	2166	0.11%	0.014%
92	14.074	4036	4038	4042	rVB5	1821	1029	0.05%	0.007%
93	14.103	4042	4047	4048	rBV4	2340	2038	0.10%	0.013%
94	14.145	4057	4060	4061	rBV3	1671	893	0.05%	0.006%
95	14.209	4076	4080	4083	rBV5	2024	2000	0.10%	0.013%
96	14.260	4093	4096	4097	rBV3	2057	990	0.05%	0.006%
97	14.334	4117	4119	4121	rBV2	2009	800	0.04%	0.005%
98	14.456	4155	4157	4161	rVB4	3452	1881	0.10%	0.012%
99	14.540	4180	4183	4186	rBV4	2202	1525	0.08%	0.010%
100	14.624	4206	4209	4211	rBV4	2703	1731	0.09%	0.011%


Sum of corrected areas: 15631766

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015175.D
Acq On : 26 Mar 2020 19:22
Operator : SY/MD
Sample : L2045-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

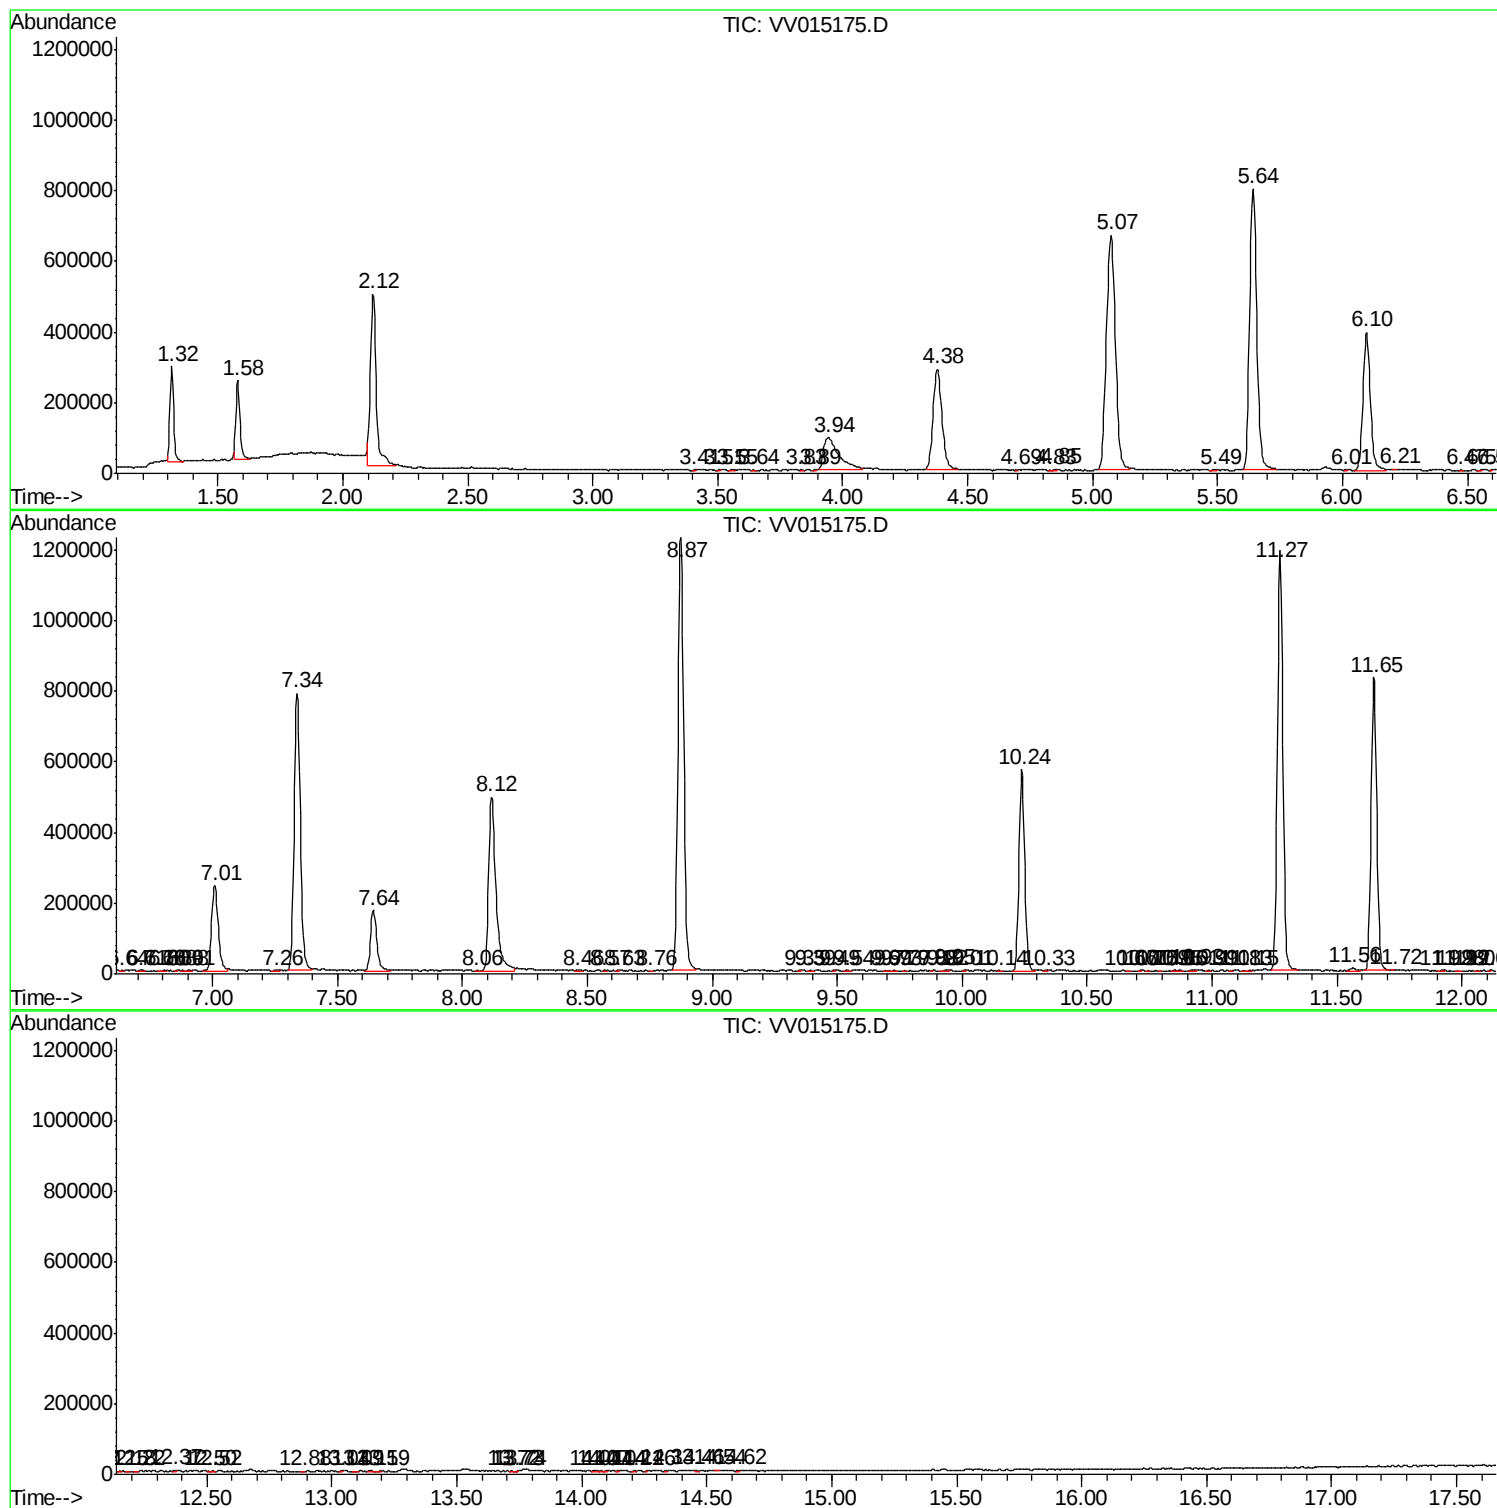

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015175.D
Acq On : 26 Mar 2020 19:22
Operator : SY/MD
Sample : L2045-03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AC0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015175.D
Acq On : 26 Mar 2020 19:22
Operator : SY/MD
Sample : L2045-03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AC0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc