

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015177.D
 Acq On : 26 Mar 2020 20:11
 Operator : SY/MD
 Sample : L1941-13RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC4RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	263550	260166	13.24%	1.648%
2	1.579	147	152	165	rVB	231483	252421	12.84%	1.599%
3	2.119	314	320	345	rVB	495418	769517	39.16%	4.874%
4	3.576	769	773	776	rBV4	2358	1910	0.10%	0.012%
5	3.592	776	778	783	rBV4	1480	1138	0.06%	0.007%
6	3.752	826	828	831	rBV4	1579	780	0.04%	0.005%
7	3.814	844	847	848	rBV3	2928	1507	0.08%	0.010%
8	3.942	875	887	922	rBV	89922	387104	19.70%	2.452%
9	4.379	1008	1023	1043	rBV	287679	707161	35.99%	4.479%
10	4.961	1202	1204	1206	rBV2	1624	713	0.04%	0.005%
11	4.990	1210	1213	1214	rBV2	1928	1181	0.06%	0.007%
12	5.074	1222	1239	1265	rBV2	670358	1674979	85.23%	10.608%
13	5.643	1403	1416	1450	rBV	782344	1557014	79.23%	9.861%
14	6.096	1545	1557	1578	rVB	388750	778412	39.61%	4.930%
15	6.537	1692	1694	1700	rVB6	2325	1658	0.08%	0.011%
16	6.627	1720	1722	1724	rBV3	1205	671	0.03%	0.004%
17	6.678	1736	1738	1741	rBV3	1987	1430	0.07%	0.009%
18	6.749	1757	1760	1761	rBV2	2667	1519	0.08%	0.010%
19	6.778	1766	1769	1770	rBV3	2583	1329	0.07%	0.008%
20	6.794	1770	1774	1777	rVB6	2074	1493	0.08%	0.009%
21	6.836	1783	1787	1788	rBV4	2356	1557	0.08%	0.010%
22	6.916	1809	1812	1813	rBV3	1381	883	0.04%	0.006%
23	6.945	1820	1821	1825	rVB4	1343	854	0.04%	0.005%
24	7.010	1830	1841	1859	rVV	241313	430561	21.91%	2.727%
25	7.286	1925	1927	1929	rBV3	1855	817	0.04%	0.005%
26	7.338	1930	1943	1962	rBV	785043	1361167	69.27%	8.621%
27	7.643	2028	2038	2051	rBV	171690	284036	14.45%	1.799%
28	7.894	2115	2116	2117	rBV	861	291	0.01%	0.002%
29	8.116	2175	2185	2207	rBV2	489314	976215	49.68%	6.183%
30	8.421	2276	2280	2284	rBV7	3097	3216	0.16%	0.020%
31	8.556	2319	2322	2329	rBV7	2660	3195	0.16%	0.020%
32	8.874	2405	2421	2441	rBV	1197249	1965137	100.00%	12.446%
33	9.328	2560	2562	2564	rVB3	1487	521	0.03%	0.003%
34	9.341	2564	2566	2573	rVB9	3495	3244	0.17%	0.021%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015177.D
 Acq On : 26 Mar 2020 20:11
 Operator : SY/MD
 Sample : L1941-13RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC4RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	9.373	2573	2576	2578	rBV4	3068	2554	0.13%	0.016%
36	9.450	2598	2600	2601	rBV2	1641	703	0.04%	0.004%
37	9.698	2675	2677	2678	rBV2	1034	340	0.02%	0.002%
38	9.710	2678	2681	2686	rVB6	2831	2321	0.12%	0.015%
39	9.733	2686	2688	2689	rBV2	1216	438	0.02%	0.003%
40	10.067	2789	2792	2795	rBV5	2366	1781	0.09%	0.011%
41	10.106	2802	2804	2805	rBV2	1481	772	0.04%	0.005%
42	10.148	2814	2817	2823	rVB8	2698	3045	0.15%	0.019%
43	10.186	2826	2829	2831	rVV4	2919	1524	0.08%	0.010%
44	10.238	2833	2845	2865	rBV	554692	894993	45.54%	5.668%
45	10.540	2936	2939	2942	rBV5	2353	2181	0.11%	0.014%
46	10.833	3026	3030	3034	rBV7	2204	1825	0.09%	0.012%
47	10.903	3049	3052	3054	rBV4	1307	1140	0.06%	0.007%
48	10.974	3070	3074	3077	rBV5	2087	1765	0.09%	0.011%
49	11.206	3138	3146	3155	rBV2	22215	34783	1.77%	0.220%
50	11.270	3155	3166	3186	rVV	1168535	1863272	94.82%	11.801%
51	11.453	3221	3223	3226	rBV4	1751	865	0.04%	0.005%
52	11.649	3272	3284	3300	rBV	850957	1360782	69.25%	8.618%
53	11.993	3389	3391	3392	rBV2	1915	912	0.05%	0.006%
54	12.273	3472	3478	3485	rBV7	5221	7173	0.37%	0.045%
55	12.357	3501	3504	3506	rBV3	2069	1346	0.07%	0.009%
56	12.440	3528	3530	3531	rBV2	1178	577	0.03%	0.004%
57	12.575	3571	3572	3576	rBV4	1813	1408	0.07%	0.009%
58	12.932	3680	3683	3687	rBV5	1823	1445	0.07%	0.009%
59	13.209	3765	3769	3775	rVB8	2486	2586	0.13%	0.016%
60	13.238	3775	3778	3781	rBV4	1567	1319	0.07%	0.008%
61	13.286	3784	3793	3803	rBV2	71356	113291	5.77%	0.717%
62	13.646	3900	3905	3909	rBV6	3405	3613	0.18%	0.023%
63	13.768	3938	3943	3954	rVB2	32330	47206	2.40%	0.299%


Sum of corrected areas: 15789757

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015177.D
Acq On : 26 Mar 2020 20:11
Operator : SY/MD
Sample : L1941-13RE
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC4RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

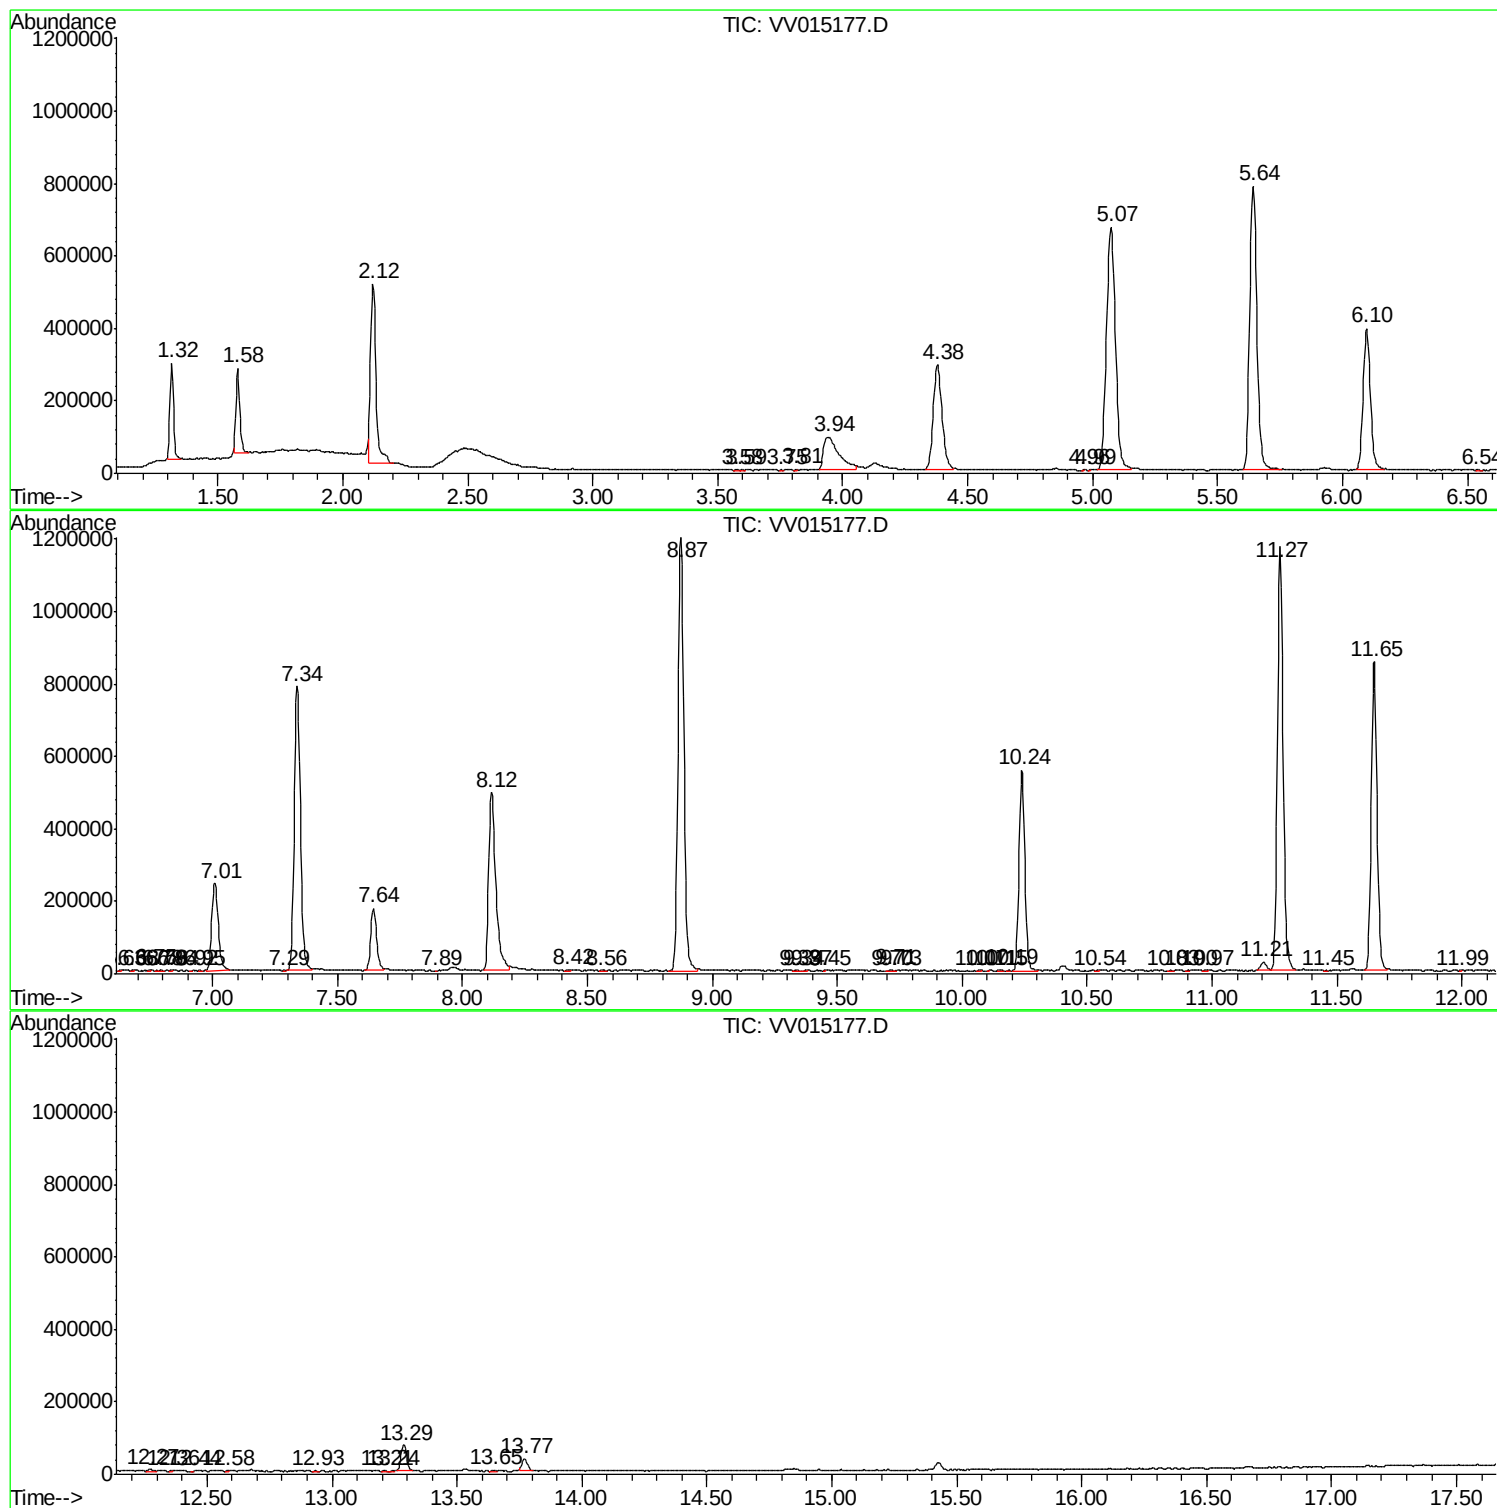

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015177.D
Acq On : 26 Mar 2020 20:11
Operator : SY/MD
Sample : L1941-13RE
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DC4RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015177.D
Acq On : 26 Mar 2020 20:11
Operator : SY/MD
Sample : L1941-13RE
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DC4RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc