

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015178.D
 Acq On : 26 Mar 2020 20:35
 Operator : SY/MD
 Sample : L1941-14RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC5RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	80	rVB	254800	258200	10.05%	1.536%
2	1.579	146	152	163	rBV	222149	261862	10.19%	1.558%
3	2.119	314	320	334	rVB	466771	657967	25.61%	3.915%
4	3.402	715	719	722	rBV5	2475	1930	0.08%	0.011%
5	3.425	722	726	728	rVV5	2520	1869	0.07%	0.011%
6	3.454	732	735	739	rVV5	2582	2039	0.08%	0.012%
7	3.569	769	771	775	rBV5	1369	944	0.04%	0.006%
8	3.836	851	854	857	rVV5	2066	1218	0.05%	0.007%
9	3.852	857	859	867	rVB8	2500	2304	0.09%	0.014%
10	3.939	874	886	930	rBV	94648	422709	16.45%	2.515%
11	4.376	1008	1022	1044	rBV	281858	696703	27.12%	4.145%
12	4.926	1189	1193	1194	rBV4	1889	1249	0.05%	0.007%
13	5.074	1220	1239	1267	rBV2	668715	1679319	65.36%	9.992%
14	5.640	1403	1415	1451	rBV	775930	1536151	59.79%	9.140%
15	5.875	1485	1488	1489	rBV3	1990	1066	0.04%	0.006%
16	5.929	1495	1505	1520	rBV3	8351	20408	0.79%	0.121%
17	6.097	1545	1557	1580	rVB	391704	782439	30.45%	4.655%
18	6.312	1621	1624	1625	rBV3	1316	686	0.03%	0.004%
19	6.418	1655	1657	1659	rBV3	2620	1421	0.06%	0.008%
20	6.521	1685	1689	1692	rBV4	1081	1157	0.05%	0.007%
21	6.817	1778	1781	1785	rBV6	1890	1444	0.06%	0.009%
22	6.871	1794	1798	1800	rBV4	2029	1506	0.06%	0.009%
23	7.010	1830	1841	1860	rBV2	238387	424637	16.53%	2.527%
24	7.293	1927	1929	1931	rBV3	2219	1110	0.04%	0.007%
25	7.338	1931	1943	1968	rVV	803629	1384684	53.89%	8.239%
26	7.643	2028	2038	2055	rBV	170500	288184	11.22%	1.715%
27	7.756	2072	2073	2077	rVB3	2095	858	0.03%	0.005%
28	7.945	2125	2132	2133	rBV7	4439	4065	0.16%	0.024%
29	8.116	2174	2185	2218	rBV2	496892	1034354	40.26%	6.154%
30	8.434	2280	2284	2288	rBV6	1926	1735	0.07%	0.010%
31	8.476	2295	2297	2299	rBV3	1613	598	0.02%	0.004%
32	8.537	2314	2316	2319	rBV4	1348	603	0.02%	0.004%
33	8.617	2338	2341	2345	rVB7	2164	1493	0.06%	0.009%
34	8.675	2357	2359	2361	rBV3	1604	836	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015178.D
 Acq On : 26 Mar 2020 20:35
 Operator : SY/MD
 Sample : L1941-14RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC5RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	8.875	2408	2421	2452	rBV2	1214454	2569327	100.00%	15.287%
36	9.241	2532	2535	2537	rBV3	2130	1244	0.05%	0.007%
37	9.286	2546	2549	2550	rBV3	2126	1153	0.04%	0.007%
38	9.354	2567	2570	2572	rBV5	1717	1032	0.04%	0.006%
39	9.389	2578	2581	2584	rBV5	1981	1573	0.06%	0.009%
40	9.421	2590	2591	2593	rBV2	1341	650	0.03%	0.004%
41	9.469	2604	2606	2609	rVB3	1291	542	0.02%	0.003%
42	9.502	2614	2616	2617	rBV2	934	422	0.02%	0.003%
43	9.659	2662	2665	2669	rBV5	1710	1509	0.06%	0.009%
44	9.707	2678	2680	2684	rBV5	1985	1516	0.06%	0.009%
45	9.762	2695	2697	2698	rBV2	1423	491	0.02%	0.003%
46	9.939	2748	2752	2754	rBV4	1877	1767	0.07%	0.011%
47	10.048	2779	2786	2787	rBV6	2715	2826	0.11%	0.017%
48	10.077	2790	2795	2796	rBV6	2377	1886	0.07%	0.011%
49	10.180	2825	2827	2830	rVB3	706	398	0.02%	0.002%
50	10.238	2834	2845	2858	rVV	579283	910106	35.42%	5.415%
51	10.537	2935	2938	2939	rBV3	1010	535	0.02%	0.003%
52	10.550	2939	2942	2944	rBV4	1717	1260	0.05%	0.007%
53	10.727	2995	2997	2998	rBV2	905	307	0.01%	0.002%
54	10.756	3003	3006	3009	rBV5	2367	2027	0.08%	0.012%
55	10.836	3029	3031	3032	rBV3	1232	654	0.03%	0.004%
56	10.874	3039	3043	3047	rBV6	1973	1933	0.08%	0.012%
57	11.083	3102	3108	3110	rBV6	1878	1367	0.05%	0.008%
58	11.129	3120	3122	3125	rBV4	2194	1376	0.05%	0.008%
59	11.209	3131	3147	3155	rBV4	14775	28716	1.12%	0.171%
60	11.273	3155	3167	3188	rVV	1182906	1831364	71.28%	10.896%
61	11.530	3244	3247	3250	rBV5	2447	1721	0.07%	0.010%
62	11.649	3272	3284	3307	rBV2	891351	1598488	62.21%	9.511%
63	11.868	3350	3352	3354	rBV3	1301	885	0.03%	0.005%
64	11.945	3372	3376	3378	rBV5	1678	1411	0.05%	0.008%
65	11.984	3385	3388	3391	rBV5	1283	1049	0.04%	0.006%
66	12.003	3391	3394	3397	rVB4	2808	1774	0.07%	0.011%
67	12.096	3421	3423	3426	rBV3	2136	1152	0.04%	0.007%
68	12.112	3426	3428	3430	rBV4	1094	615	0.02%	0.004%
69	12.167	3441	3445	3448	rVB4	1843	1262	0.05%	0.008%
70	12.186	3448	3451	3455	rBV6	2077	2178	0.08%	0.013%
71	12.231	3462	3465	3468	rBV4	1722	1152	0.04%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015178.D
 Acq On : 26 Mar 2020 20:35
 Operator : SY/MD
 Sample : L1941-14RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC5RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	12.251	3468	3471	3473	rBV4	2011	1385	0.05%	0.008%
73	12.344	3498	3500	3504	rBV4	1522	1305	0.05%	0.008%
74	12.408	3519	3520	3521	rBV	795	188	0.01%	0.001%
75	12.418	3521	3523	3525	rBV3	1432	810	0.03%	0.005%
76	12.463	3533	3537	3540	rBV6	2188	1958	0.08%	0.012%
77	12.569	3568	3570	3571	rBV2	949	425	0.02%	0.003%
78	12.669	3595	3601	3609	rBV2	6241	10079	0.39%	0.060%
79	13.006	3703	3706	3710	rBV5	1956	1684	0.07%	0.010%
80	13.058	3719	3722	3724	rBV3	1755	1190	0.05%	0.007%
81	13.122	3739	3742	3745	rVB4	1972	1247	0.05%	0.007%
82	13.141	3745	3748	3750	rBV3	1731	1249	0.05%	0.007%
83	13.177	3757	3759	3761	rBV3	1950	1280	0.05%	0.008%
84	13.286	3783	3793	3806	rBV	134591	205922	8.01%	1.225%
85	13.392	3824	3826	3827	rBV2	1638	684	0.03%	0.004%
86	13.437	3836	3840	3841	rBV4	1535	1064	0.04%	0.006%
87	13.521	3862	3866	3867	rBV4	2785	1929	0.08%	0.011%
88	13.723	3925	3929	3931	rBV5	2044	1580	0.06%	0.009%
89	13.768	3931	3943	3955	rVV	53938	92230	3.59%	0.549%
90	13.997	4011	4014	4022	rVB10	2575	2841	0.11%	0.017%
91	14.154	4061	4063	4066	rBV3	1719	807	0.03%	0.005%
92	14.299	4105	4108	4110	rBV3	2167	1219	0.05%	0.007%
93	14.829	4262	4273	4277	rBV3	11420	20804	0.81%	0.124%


Sum of corrected areas: 16807296

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015178.D
Acq On : 26 Mar 2020 20:35
Operator : SY/MD
Sample : L1941-14RE
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC5RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

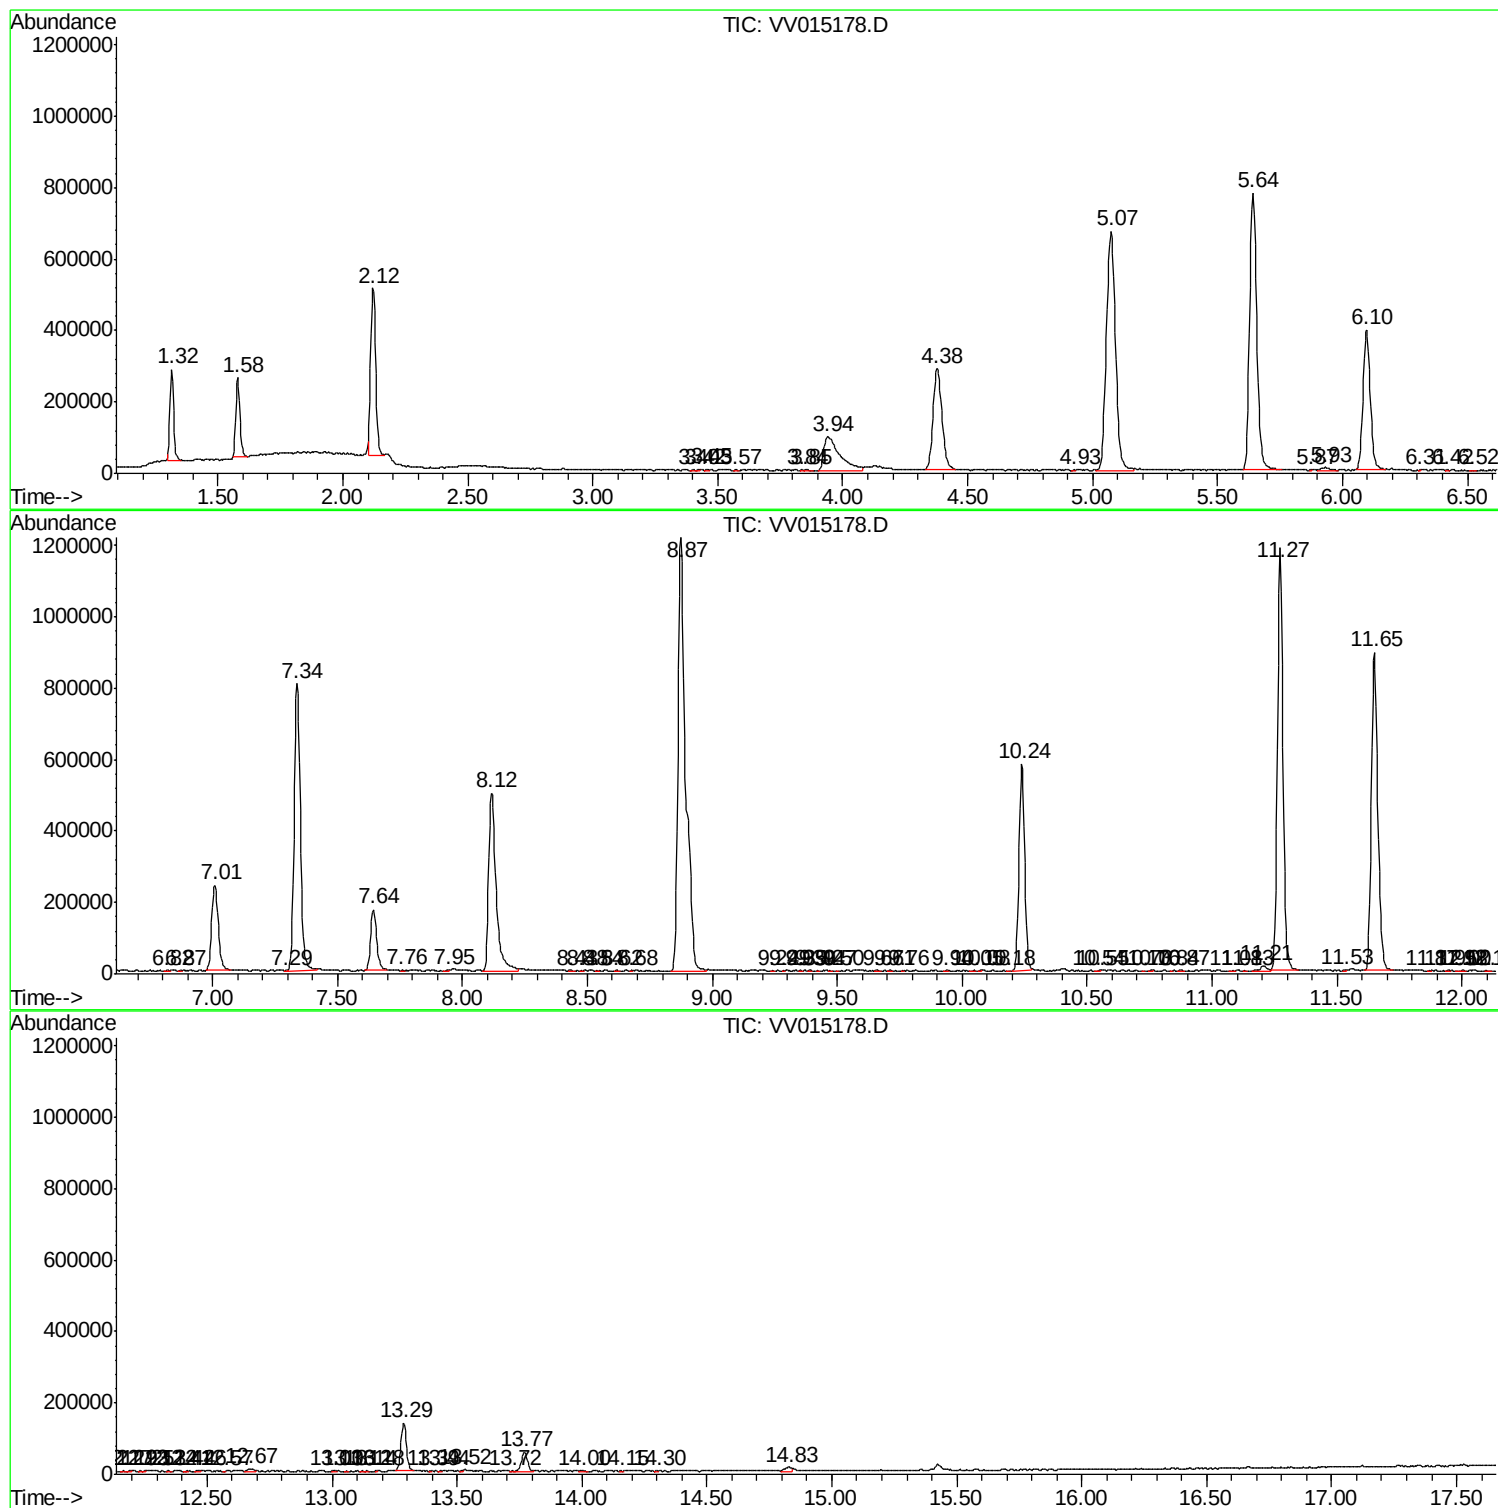

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015178.D
Acq On : 26 Mar 2020 20:35
Operator : SY/MD
Sample : L1941-14RE
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DC5RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015178.D
Acq On : 26 Mar 2020 20:35
Operator : SY/MD
Sample : L1941-14RE
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DC5RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc