

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015179.D
 Acq On : 26 Mar 2020 20:59
 Operator : SY/MD
 Sample : L1941-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	82	rVB	268421	259951	9.55%	1.334%
2	1.579	147	152	164	rVB	227745	255866	9.40%	1.313%
3	2.119	314	320	345	rVB	506031	792528	29.11%	4.067%
4	2.900	561	563	566	rBV4	2304	1741	0.06%	0.009%
5	3.003	593	595	598	rBV3	2094	1191	0.04%	0.006%
6	3.135	634	636	637	rBV2	1868	836	0.03%	0.004%
7	3.502	746	750	755	rBV7	2231	2357	0.09%	0.012%
8	3.540	758	762	765	rBV6	1636	1427	0.05%	0.007%
9	3.576	770	773	775	rBV3	2306	1286	0.05%	0.007%
10	3.746	824	826	831	rVB6	1544	923	0.03%	0.005%
11	3.801	840	843	848	rVB6	1759	1562	0.06%	0.008%
12	3.843	854	856	858	rBV2	1566	928	0.03%	0.005%
13	3.942	875	887	913	rBV2	87282	361375	13.27%	1.855%
14	4.379	1009	1023	1051	rVB	286355	713679	26.21%	3.662%
15	4.614	1092	1096	1098	rBV3	1935	1252	0.05%	0.006%
16	4.756	1138	1140	1143	rBV4	1785	900	0.03%	0.005%
17	4.942	1195	1198	1203	rVB7	1977	1502	0.06%	0.008%
18	5.074	1221	1239	1253	rBV2	682532	1716276	63.04%	8.808%
19	5.408	1341	1343	1348	rBV5	2542	1979	0.07%	0.010%
20	5.486	1365	1367	1371	rBV6	1803	1406	0.05%	0.007%
21	5.550	1385	1387	1389	rBV3	2513	1223	0.04%	0.006%
22	5.588	1396	1399	1401	rBV4	1871	1299	0.05%	0.007%
23	5.643	1403	1416	1444	rVV	764533	1535348	56.39%	7.879%
24	5.797	1461	1464	1468	rBV6	1883	1387	0.05%	0.007%
25	6.096	1543	1557	1576	rBV	403732	817586	30.03%	4.196%
26	6.341	1630	1633	1637	rBV6	1760	1070	0.04%	0.005%
27	6.370	1637	1642	1644	rBV6	1820	1896	0.07%	0.010%
28	6.489	1677	1679	1681	rBV3	1714	1042	0.04%	0.005%
29	6.531	1690	1692	1695	rVB4	1621	844	0.03%	0.004%
30	6.579	1705	1707	1709	rBV3	1569	951	0.03%	0.005%
31	6.656	1726	1731	1733	rBV5	2077	1773	0.07%	0.009%
32	6.765	1760	1765	1770	rBV8	2041	2716	0.10%	0.014%
33	6.868	1794	1797	1799	rVB3	2271	1273	0.05%	0.007%
34	6.887	1799	1803	1806	rVB7	2412	1682	0.06%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015179.D
 Acq On : 26 Mar 2020 20:59
 Operator : SY/MD
 Sample : L1941-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	6.971	1824	1829	1830	rBV4	1768	1475	0.05%	0.008%
36	7.010	1830	1841	1859	rVV	240772	433397	15.92%	2.224%
37	7.231	1907	1910	1913	rVB5	1930	1171	0.04%	0.006%
38	7.338	1931	1943	1965	rBV	813683	1409717	51.78%	7.234%
39	7.643	2029	2038	2055	rBV	172553	285846	10.50%	1.467%
40	7.965	2129	2138	2143	rBV6	7745	12940	0.48%	0.066%
41	8.035	2158	2160	2162	rBV3	1802	1102	0.04%	0.006%
42	8.116	2175	2185	2216	rBV3	500881	1030427	37.85%	5.288%
43	8.434	2282	2284	2286	rBV3	2135	1161	0.04%	0.006%
44	8.502	2300	2305	2308	rBV6	2363	1764	0.06%	0.009%
45	8.559	2321	2323	2325	rBV3	1526	898	0.03%	0.005%
46	8.649	2346	2351	2352	rBV5	2809	2499	0.09%	0.013%
47	8.717	2367	2372	2373	rBV4	2004	1521	0.06%	0.008%
48	8.874	2404	2421	2450	rBV2	1220031	2722626	100.00%	13.972%
49	9.222	2525	2529	2533	rVB6	2014	1475	0.05%	0.008%
50	9.337	2563	2565	2567	rBV3	1878	940	0.03%	0.005%
51	9.450	2598	2600	2605	rVB6	1456	1140	0.04%	0.006%
52	9.566	2628	2636	2637	rBV7	3787	4287	0.16%	0.022%
53	9.643	2656	2660	2664	rBV6	1467	1535	0.06%	0.008%
54	9.720	2680	2684	2686	rBV5	1610	1302	0.05%	0.007%
55	9.868	2728	2730	2736	rVB7	2365	1846	0.07%	0.009%
56	9.900	2736	2740	2742	rBV4	1521	1316	0.05%	0.007%
57	10.038	2779	2783	2786	rBV5	1561	1376	0.05%	0.007%
58	10.145	2810	2816	2818	rBV7	1165	1267	0.05%	0.007%
59	10.238	2832	2845	2862	rBV	583358	925343	33.99%	4.749%
60	10.341	2875	2877	2881	rBV4	1516	1223	0.04%	0.006%
61	10.405	2891	2897	2908	rVB4	12004	19256	0.71%	0.099%
62	10.447	2908	2910	2912	rBV3	1709	867	0.03%	0.004%
63	10.521	2931	2933	2937	rVB5	1750	1098	0.04%	0.006%
64	10.553	2937	2943	2944	rBV5	1841	1680	0.06%	0.009%
65	10.624	2963	2965	2970	rVB5	1417	1013	0.04%	0.005%
66	10.662	2975	2977	2983	rVB6	1600	1228	0.05%	0.006%
67	10.768	3004	3010	3014	rVB8	3312	3554	0.13%	0.018%
68	10.791	3014	3017	3020	rBV4	2686	1524	0.06%	0.008%
69	10.836	3029	3031	3037	rBV7	1191	1117	0.04%	0.006%
70	10.871	3039	3042	3045	rBV5	1233	1291	0.05%	0.007%
71	10.926	3054	3059	3060	rBV5	1607	1376	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015179.D
 Acq On : 26 Mar 2020 20:59
 Operator : SY/MD
 Sample : L1941-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	10.968	3070	3072	3078	rVB6	2109	1751	0.06%	0.009%
73	11.013	3083	3086	3090	rBV6	1588	1500	0.06%	0.008%
74	11.206	3136	3146	3155	rBV3	100006	159315	5.85%	0.818%
75	11.273	3156	3167	3192	rVB2	1237301	2621434	96.28%	13.453%
76	11.511	3238	3241	3244	rBV4	1897	1065	0.04%	0.005%
77	11.649	3271	3284	3302	rBV2	1011808	2192404	80.53%	11.251%
78	11.849	3341	3346	3349	rBV5	3827	4197	0.15%	0.022%
79	11.935	3369	3373	3378	rVB8	2657	2501	0.09%	0.013%
80	11.961	3378	3381	3383	rVB4	1631	966	0.04%	0.005%
81	11.990	3386	3390	3392	rBV4	2024	1773	0.07%	0.009%
82	12.080	3416	3418	3419	rBV2	1723	839	0.03%	0.004%
83	12.212	3457	3459	3462	rVB3	2083	917	0.03%	0.005%
84	12.276	3472	3479	3485	rVB7	3604	4925	0.18%	0.025%
85	12.325	3492	3494	3499	rBV5	1587	1295	0.05%	0.007%
86	12.511	3548	3552	3553	rBV3	1723	884	0.03%	0.005%
87	12.646	3591	3594	3595	rBV2	2318	1304	0.05%	0.007%
88	12.714	3612	3615	3617	rBV3	2838	1950	0.07%	0.010%
89	12.868	3660	3663	3666	rBV5	2132	1319	0.05%	0.007%
90	13.183	3757	3761	3763	rBV5	1976	1433	0.05%	0.007%
91	13.215	3767	3771	3772	rBV4	1755	1336	0.05%	0.007%
92	13.286	3780	3793	3808	rBV	521075	807786	29.67%	4.145%
93	13.527	3863	3868	3872	rBV7	4225	5309	0.19%	0.027%
94	13.656	3906	3908	3910	rBV3	1573	912	0.03%	0.005%
95	13.669	3910	3912	3915	rVB4	1677	877	0.03%	0.005%
96	13.691	3917	3919	3921	rBV2	1484	837	0.03%	0.004%
97	13.768	3933	3943	3961	rVB	180249	287955	10.58%	1.478%
98	14.209	4077	4080	4084	rVB5	3079	1789	0.07%	0.009%
99	14.289	4101	4105	4107	rBV5	2325	1997	0.07%	0.010%
100	14.514	4170	4175	4177	rBV5	3289	3138	0.12%	0.016%


Sum of corrected areas: 19486361

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015179.D
Acq On : 26 Mar 2020 20:59
Operator : SY/MD
Sample : L1941-18
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0DL8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

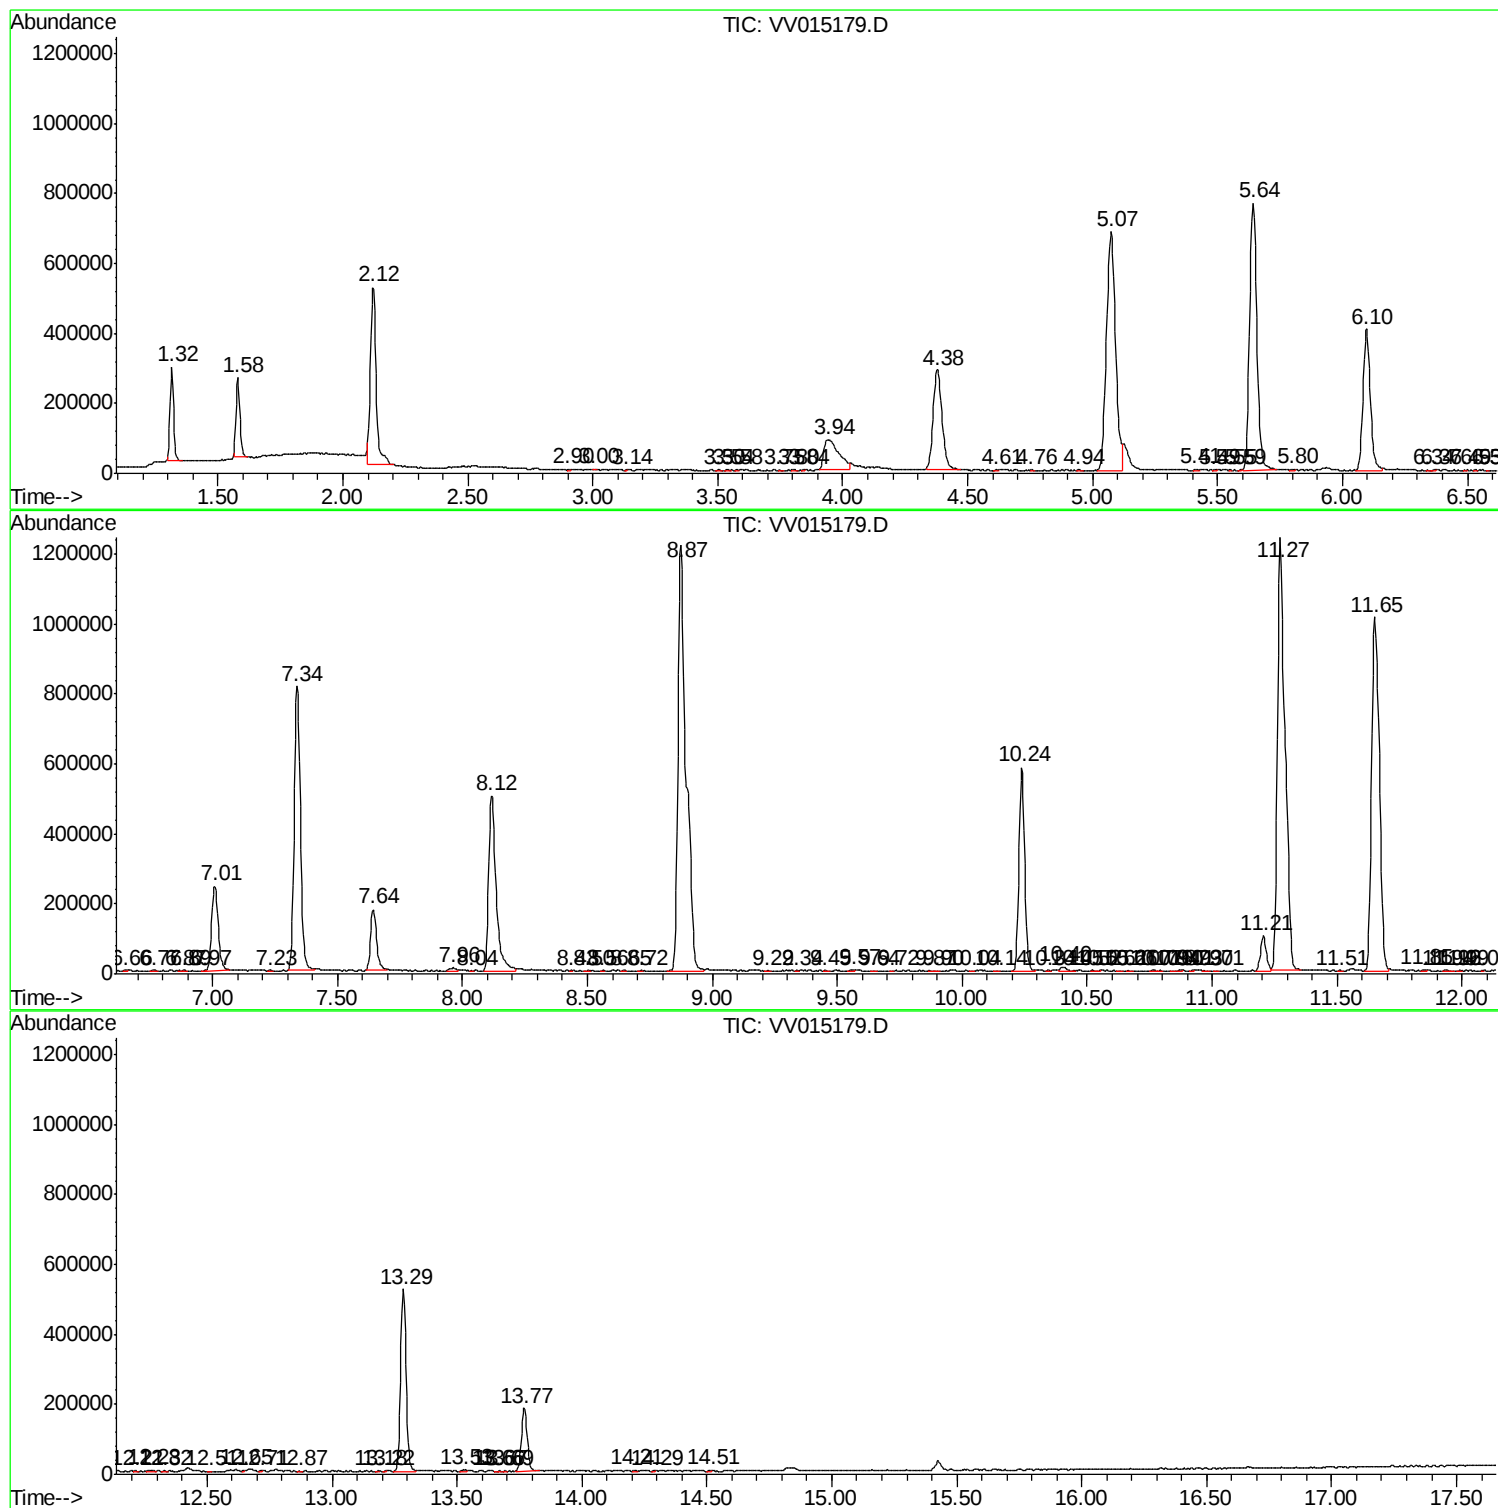

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015179.D
Acq On : 26 Mar 2020 20:59
Operator : SY/MD
Sample : L1941-18
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DL8

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015179.D
Acq On : 26 Mar 2020 20:59
Operator : SY/MD
Sample : L1941-18
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DL8

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc