

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015180.D
 Acq On : 26 Mar 2020 21:24
 Operator : SY/MD
 Sample : L2045-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	281114	283686	15.16%	1.851%
2	2.119	314	320	342	rVB	488539	741616	39.62%	4.838%
3	3.026	600	602	604	rBV3	2569	1592	0.09%	0.010%
4	3.389	714	715	719	rBV3	951	591	0.03%	0.004%
5	3.502	748	750	752	rBV3	656	296	0.02%	0.002%
6	3.724	817	819	820	rBV2	1394	642	0.03%	0.004%
7	3.766	830	832	833	rBV2	1273	466	0.02%	0.003%
8	3.801	840	843	847	rBV6	1987	1567	0.08%	0.010%
9	3.942	874	887	911	rBV2	99332	397441	21.24%	2.593%
10	4.380	1010	1023	1042	rVB	278744	666730	35.62%	4.349%
11	4.846	1166	1168	1173	rVB5	2204	1208	0.06%	0.008%
12	4.888	1180	1181	1183	rVB2	820	307	0.02%	0.002%
13	4.901	1183	1185	1186	rBV2	1362	604	0.03%	0.004%
14	4.917	1187	1190	1192	rVV4	1709	1007	0.05%	0.007%
15	4.974	1206	1208	1210	rVB3	1377	503	0.03%	0.003%
16	5.074	1222	1239	1262	rBV2	665910	1658201	88.60%	10.817%
17	5.360	1325	1328	1331	rBV5	1375	1330	0.07%	0.009%
18	5.640	1402	1415	1442	rBV	758813	1518071	81.11%	9.903%
19	5.794	1461	1463	1466	rBV3	1682	1159	0.06%	0.008%
20	5.846	1477	1479	1485	rVB7	1645	768	0.04%	0.005%
21	6.097	1544	1557	1582	rVB	389697	795262	42.49%	5.188%
22	6.232	1591	1599	1609	rBV9	8238	16173	0.86%	0.106%
23	6.447	1664	1666	1667	rBV2	1794	748	0.04%	0.005%
24	6.508	1683	1685	1686	rBV2	1321	539	0.03%	0.004%
25	6.569	1702	1704	1706	rBV3	886	290	0.02%	0.002%
26	6.582	1706	1708	1709	rBV2	1342	561	0.03%	0.004%
27	6.621	1716	1720	1722	rBV5	1623	1342	0.07%	0.009%
28	6.720	1747	1751	1755	rVB6	1667	1675	0.09%	0.011%
29	6.878	1796	1800	1803	rBV5	1999	1341	0.07%	0.009%
30	6.894	1803	1805	1807	rBV2	1602	723	0.04%	0.005%
31	6.965	1823	1827	1829	rBV5	2001	1607	0.09%	0.010%
32	7.010	1829	1841	1860	rVV	237114	435448	23.27%	2.841%
33	7.164	1886	1889	1891	rBV4	1605	884	0.05%	0.006%
34	7.180	1891	1894	1896	rBV4	2072	1412	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015180.D
 Acq On : 26 Mar 2020 21:24
 Operator : SY/MD
 Sample : L2045-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	7.257	1909	1918	1931	rBV2	77906	144051	7.70%	0.940%
36	7.338	1932	1943	1960	rVV	767359	1318525	70.45%	8.601%
37	7.643	2029	2038	2054	rVB	170143	281632	15.05%	1.837%
38	7.859	2102	2105	2106	rBV3	2112	1215	0.06%	0.008%
39	8.116	2173	2185	2213	rBV2	540271	1105917	59.09%	7.214%
40	8.527	2311	2313	2318	rBV6	2045	1533	0.08%	0.010%
41	8.582	2326	2330	2333	rBV6	2030	2055	0.11%	0.013%
42	8.675	2358	2359	2361	rVB2	864	218	0.01%	0.001%
43	8.688	2361	2363	2365	rBV2	1950	1219	0.07%	0.008%
44	8.752	2376	2383	2385	rBV7	2710	3100	0.17%	0.020%
45	8.788	2392	2394	2396	rBV3	2034	1047	0.06%	0.007%
46	8.875	2408	2421	2444	rBV	1156741	1871630	100.00%	12.209%
47	9.505	2614	2617	2618	rBV3	1473	892	0.05%	0.006%
48	9.569	2630	2637	2643	rBV2	8103	11983	0.64%	0.078%
49	9.666	2663	2667	2671	rVB6	1628	1680	0.09%	0.011%
50	10.019	2775	2777	2778	rBV2	2028	940	0.05%	0.006%
51	10.071	2785	2793	2797	rBV10	4272	4827	0.26%	0.031%
52	10.135	2811	2813	2816	rBV4	1592	872	0.05%	0.006%
53	10.151	2816	2818	2819	rBV2	1837	598	0.03%	0.004%
54	10.238	2836	2845	2865	rVB	599706	954075	50.98%	6.224%
55	10.363	2882	2884	2886	rBV3	1827	1037	0.06%	0.007%
56	10.540	2935	2939	2941	rBV5	3319	2595	0.14%	0.017%
57	10.669	2977	2979	2983	rBV5	1710	1103	0.06%	0.007%
58	10.723	2989	2996	3001	rBV9	8867	12836	0.69%	0.084%
59	11.270	3156	3166	3190	rVB	1139513	1745755	93.27%	11.388%
60	11.649	3273	3284	3301	rVB	819116	1275580	68.15%	8.321%
61	12.074	3412	3416	3424	rBV8	5608	8874	0.47%	0.058%
62	12.707	3610	3613	3615	rVB4	2136	1220	0.07%	0.008%
63	12.730	3615	3620	3622	rBV6	2625	2492	0.13%	0.016%
64	12.759	3623	3629	3636	rVV6	8251	12559	0.67%	0.082%
65	12.965	3689	3693	3694	rBV4	2296	1729	0.09%	0.011%
66	13.116	3736	3740	3742	rBV5	2811	2235	0.12%	0.015%
67	13.836	3962	3964	3967	rVB3	1883	797	0.04%	0.005%
68	13.858	3967	3971	3974	rBV5	3711	3098	0.17%	0.020%
69	13.916	3984	3989	3990	rBV5	3220	2724	0.15%	0.018%
70	13.952	3995	4000	4008	rVV5	5559	9196	0.49%	0.060%
71	15.395	4446	4449	4450	rBV3	3219	1973	0.11%	0.013%

LSC Area Percent Report

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015180.D
Acq On : 26 Mar 2020 21:24
Operator : SY/MD
Sample : L2045-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Title : VOC Analysis


Sum of corrected areas: 15329602

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015180.D
Acq On : 26 Mar 2020 21:24
Operator : SY/MD
Sample : L2045-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

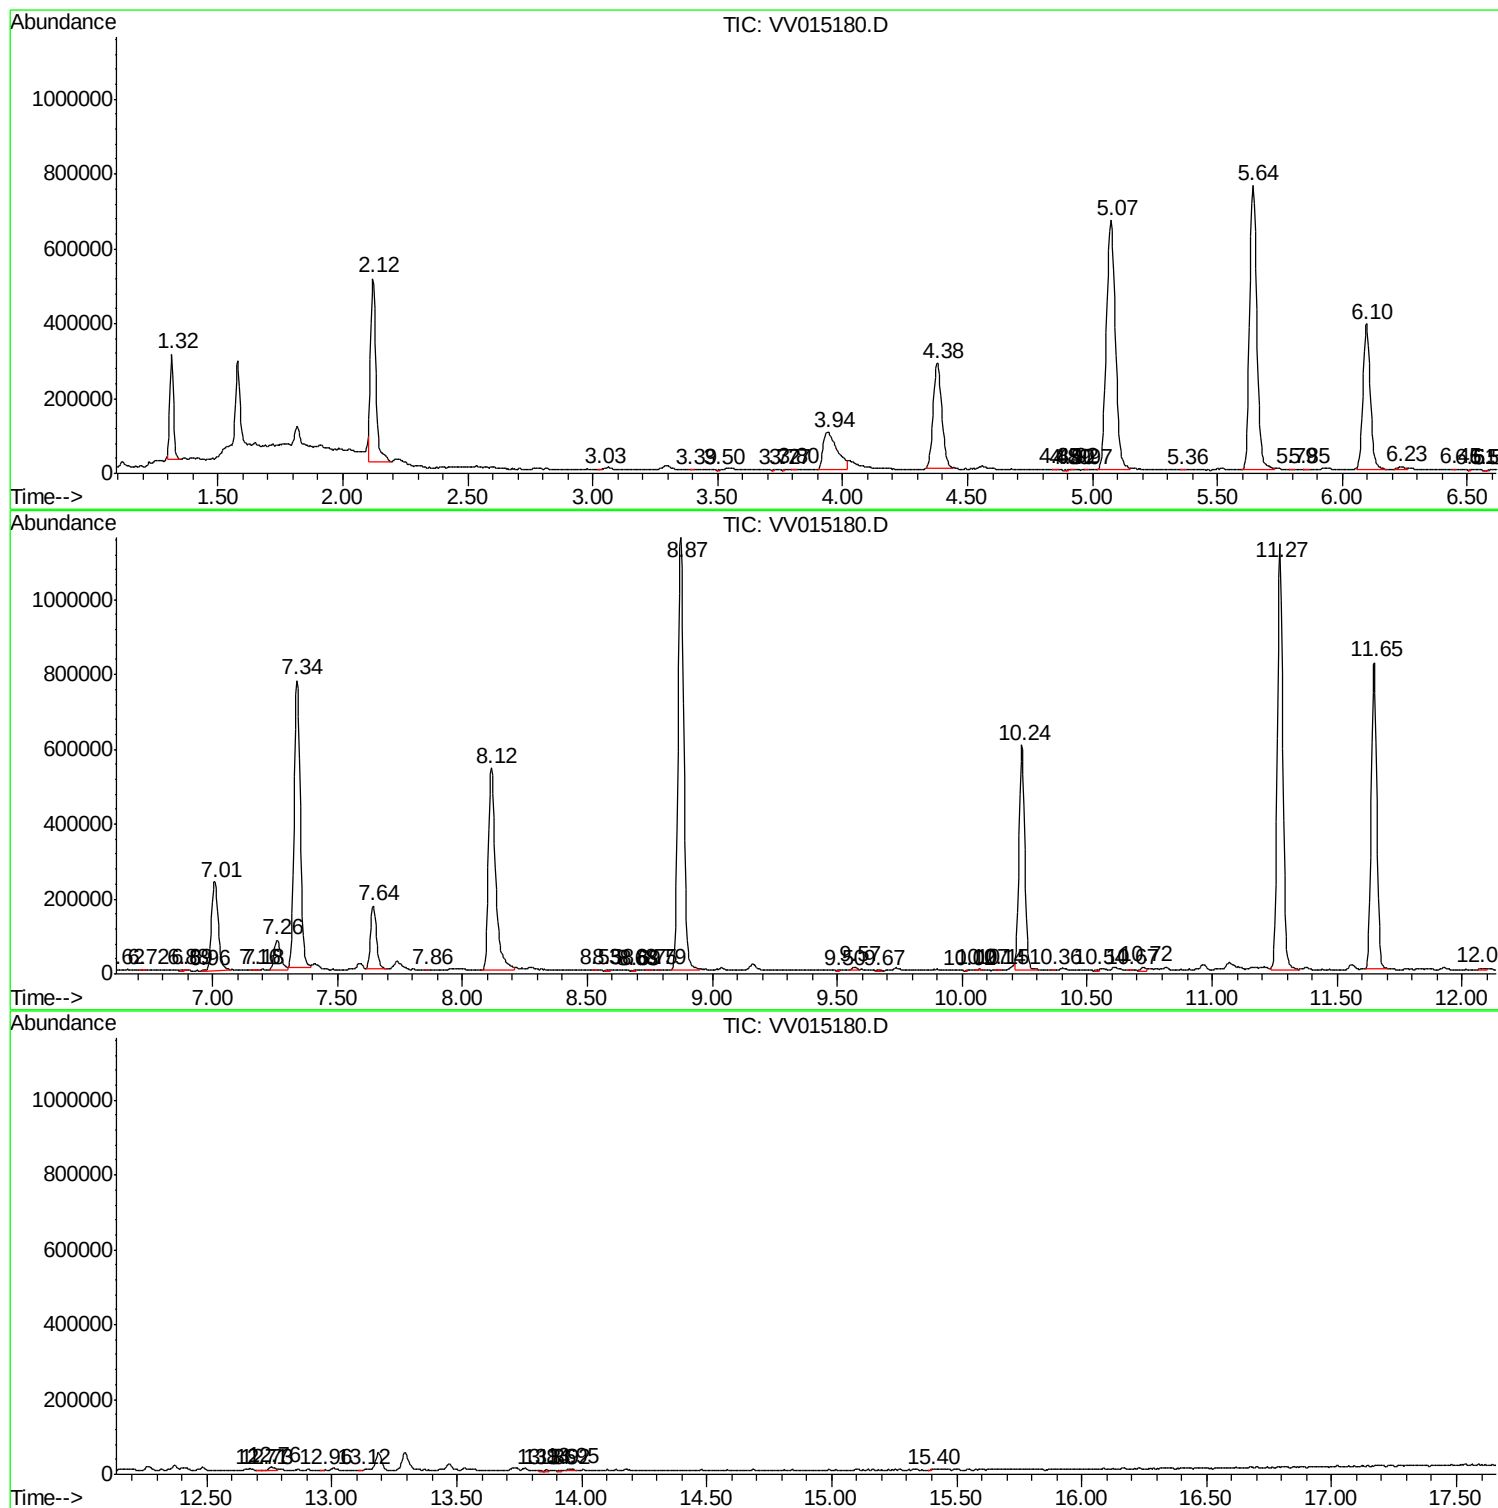

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015180.D
Acq On : 26 Mar 2020 21:24
Operator : SY/MD
Sample : L2045-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AB6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015180.D
Acq On : 26 Mar 2020 21:24
Operator : SY/MD
Sample : L2045-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AB6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc