

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015184.D
 Acq On : 26 Mar 2020 23:01
 Operator : SY/MD
 Sample : VIBLK73
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	80	rVB	251348	257157	13.46%	1.490%
2	1.579	146	152	162	rVB	236988	272228	14.25%	1.577%
3	2.119	314	320	332	rVB	445903	613846	32.12%	3.557%
4	3.251	669	672	676	rBV5	1720	1129	0.06%	0.007%
5	3.528	754	758	761	rBV4	2477	2031	0.11%	0.012%
6	3.640	790	793	794	rBV3	1537	930	0.05%	0.005%
7	3.669	799	802	804	rBV3	2331	1484	0.08%	0.009%
8	3.756	827	829	830	rBV2	2747	1183	0.06%	0.007%
9	3.897	868	873	874	rBV5	2288	1715	0.09%	0.010%
10	3.936	874	885	928	rVV	135458	598478	31.32%	3.467%
11	4.377	1002	1022	1049	rBV	334638	846956	44.32%	4.907%
12	4.962	1202	1204	1209	rBV5	1483	907	0.05%	0.005%
13	5.071	1222	1238	1264	rBV2	761135	1910889	100.00%	11.071%
14	5.569	1391	1393	1396	rBV4	1539	862	0.05%	0.005%
15	5.640	1403	1415	1441	rBV	734067	1468886	76.87%	8.510%
16	6.003	1526	1528	1530	rBV4	1368	667	0.03%	0.004%
17	6.097	1543	1557	1581	rBV	461736	943467	49.37%	5.466%
18	6.418	1654	1657	1659	rBV4	1845	1283	0.07%	0.007%
19	6.473	1670	1674	1678	rBV6	2113	2034	0.11%	0.012%
20	6.528	1688	1691	1699	rVB9	3051	2404	0.13%	0.014%
21	6.634	1720	1724	1728	rBV6	2416	2198	0.12%	0.013%
22	6.753	1758	1761	1763	rBV3	2497	1857	0.10%	0.011%
23	7.007	1829	1840	1858	rBV	279983	500409	26.19%	2.899%
24	7.338	1931	1943	1964	rBV	818947	1409988	73.79%	8.169%
25	7.540	2004	2006	2008	rBV3	1289	758	0.04%	0.004%
26	7.643	2028	2038	2050	rBV	205555	343397	17.97%	1.990%
27	7.933	2124	2128	2129	rBV4	1359	975	0.05%	0.006%
28	7.952	2132	2134	2138	rVV4	2168	1346	0.07%	0.008%
29	8.042	2159	2162	2165	rBV5	1402	1248	0.07%	0.007%
30	8.116	2174	2185	2215	rBV2	729289	1452114	75.99%	8.413%
31	8.454	2287	2290	2295	rBV7	2338	2225	0.12%	0.013%
32	8.804	2396	2399	2400	rBV3	1768	1058	0.06%	0.006%
33	8.875	2409	2421	2451	rBV	1142551	1878280	98.29%	10.882%
34	9.093	2486	2489	2492	rBV5	2100	1953	0.10%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015184.D
 Acq On : 26 Mar 2020 23:01
 Operator : SY/MD
 Sample : VIBLK73
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	9.302	2553	2554	2555	rBV	1469	515	0.03%	0.003%
36	9.341	2564	2566	2570	rVB5	1201	578	0.03%	0.003%
37	9.367	2570	2574	2577	rBV6	2346	1808	0.09%	0.010%
38	9.441	2595	2597	2599	rBV3	1256	685	0.04%	0.004%
39	9.463	2600	2604	2609	rBV8	2233	2463	0.13%	0.014%
40	9.566	2634	2636	2638	rBV3	1939	993	0.05%	0.006%
41	9.646	2658	2661	2662	rBV3	1906	927	0.05%	0.005%
42	9.791	2704	2706	2707	rBV2	1266	379	0.02%	0.002%
43	9.875	2730	2732	2734	rVB3	2174	828	0.04%	0.005%
44	9.900	2735	2740	2742	rBV6	1703	1482	0.08%	0.009%
45	10.154	2818	2819	2820	rBV	1239	314	0.02%	0.002%
46	10.238	2832	2845	2865	rBV	774397	1226191	64.17%	7.104%
47	10.408	2896	2898	2901	rVB3	2819	1175	0.06%	0.007%
48	10.518	2930	2932	2933	rBV2	1722	604	0.03%	0.003%
49	10.553	2942	2943	2946	rBV3	2309	1413	0.07%	0.008%
50	10.621	2963	2964	2967	rVB3	1855	793	0.04%	0.005%
51	10.637	2967	2969	2970	rBV2	949	244	0.01%	0.001%
52	10.675	2978	2981	2984	rBV4	2063	1291	0.07%	0.007%
53	10.701	2985	2989	2990	rVV4	1702	1163	0.06%	0.007%
54	10.804	3014	3021	3022	rBV6	1803	1900	0.10%	0.011%
55	10.994	3078	3080	3082	rBV3	946	414	0.02%	0.002%
56	11.084	3104	3108	3109	rBV3	2316	1673	0.09%	0.010%
57	11.174	3130	3136	3139	rBV8	1558	1799	0.09%	0.010%
58	11.273	3153	3167	3192	rBV	1142741	1772871	92.78%	10.272%
59	11.534	3242	3248	3252	rBV9	3682	4075	0.21%	0.024%
60	11.646	3271	3283	3305	rBV	1050671	1660606	86.90%	9.621%
61	12.116	3425	3429	3431	rBV5	1678	894	0.05%	0.005%
62	12.203	3453	3456	3459	rBV5	1470	1161	0.06%	0.007%
63	12.299	3483	3486	3488	rBV5	1965	1010	0.05%	0.006%
64	12.312	3488	3490	3492	rBV3	1026	680	0.04%	0.004%
65	12.360	3503	3505	3507	rBV2	1584	1001	0.05%	0.006%
66	12.457	3532	3535	3540	rBV5	1113	886	0.05%	0.005%
67	12.482	3540	3543	3546	rBV5	1603	1237	0.06%	0.007%
68	12.527	3553	3557	3558	rBV4	1920	1289	0.07%	0.007%
69	12.559	3564	3567	3568	rBV3	1414	949	0.05%	0.005%
70	12.662	3597	3599	3600	rBV2	1336	664	0.03%	0.004%
71	12.794	3636	3640	3642	rBV5	1656	1036	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015184.D
 Acq On : 26 Mar 2020 23:01
 Operator : SY/MD
 Sample : VIBLK73
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	12.833	3648	3652	3655	rBV6	2187	2036	0.11%	0.012%
73	12.865	3658	3662	3667	rBV7	1710	1854	0.10%	0.011%
74	12.923	3678	3680	3682	rBV3	1288	601	0.03%	0.003%
75	13.010	3704	3707	3710	rBV5	2372	1592	0.08%	0.009%
76	13.119	3738	3741	3743	rBV3	2287	1455	0.08%	0.008%
77	13.148	3748	3750	3752	rBV2	1461	620	0.03%	0.004%
78	13.257	3780	3784	3787	rBV5	2475	2114	0.11%	0.012%
79	13.289	3787	3794	3805	rVB5	10947	18304	0.96%	0.106%
80	13.331	3805	3807	3810	rBV4	1935	1254	0.07%	0.007%
81	13.412	3830	3832	3833	rBV2	2037	772	0.04%	0.004%
82	13.527	3864	3868	3869	rBV5	1920	1303	0.07%	0.008%
83	14.145	4057	4060	4063	rBV4	1930	1498	0.08%	0.009%
84	14.588	4195	4198	4201	rBV5	3144	1985	0.10%	0.012%


Sum of corrected areas: 17259721

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015184.D
Acq On : 26 Mar 2020 23:01
Operator : SY/MD
Sample : VIBLK73
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK73

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

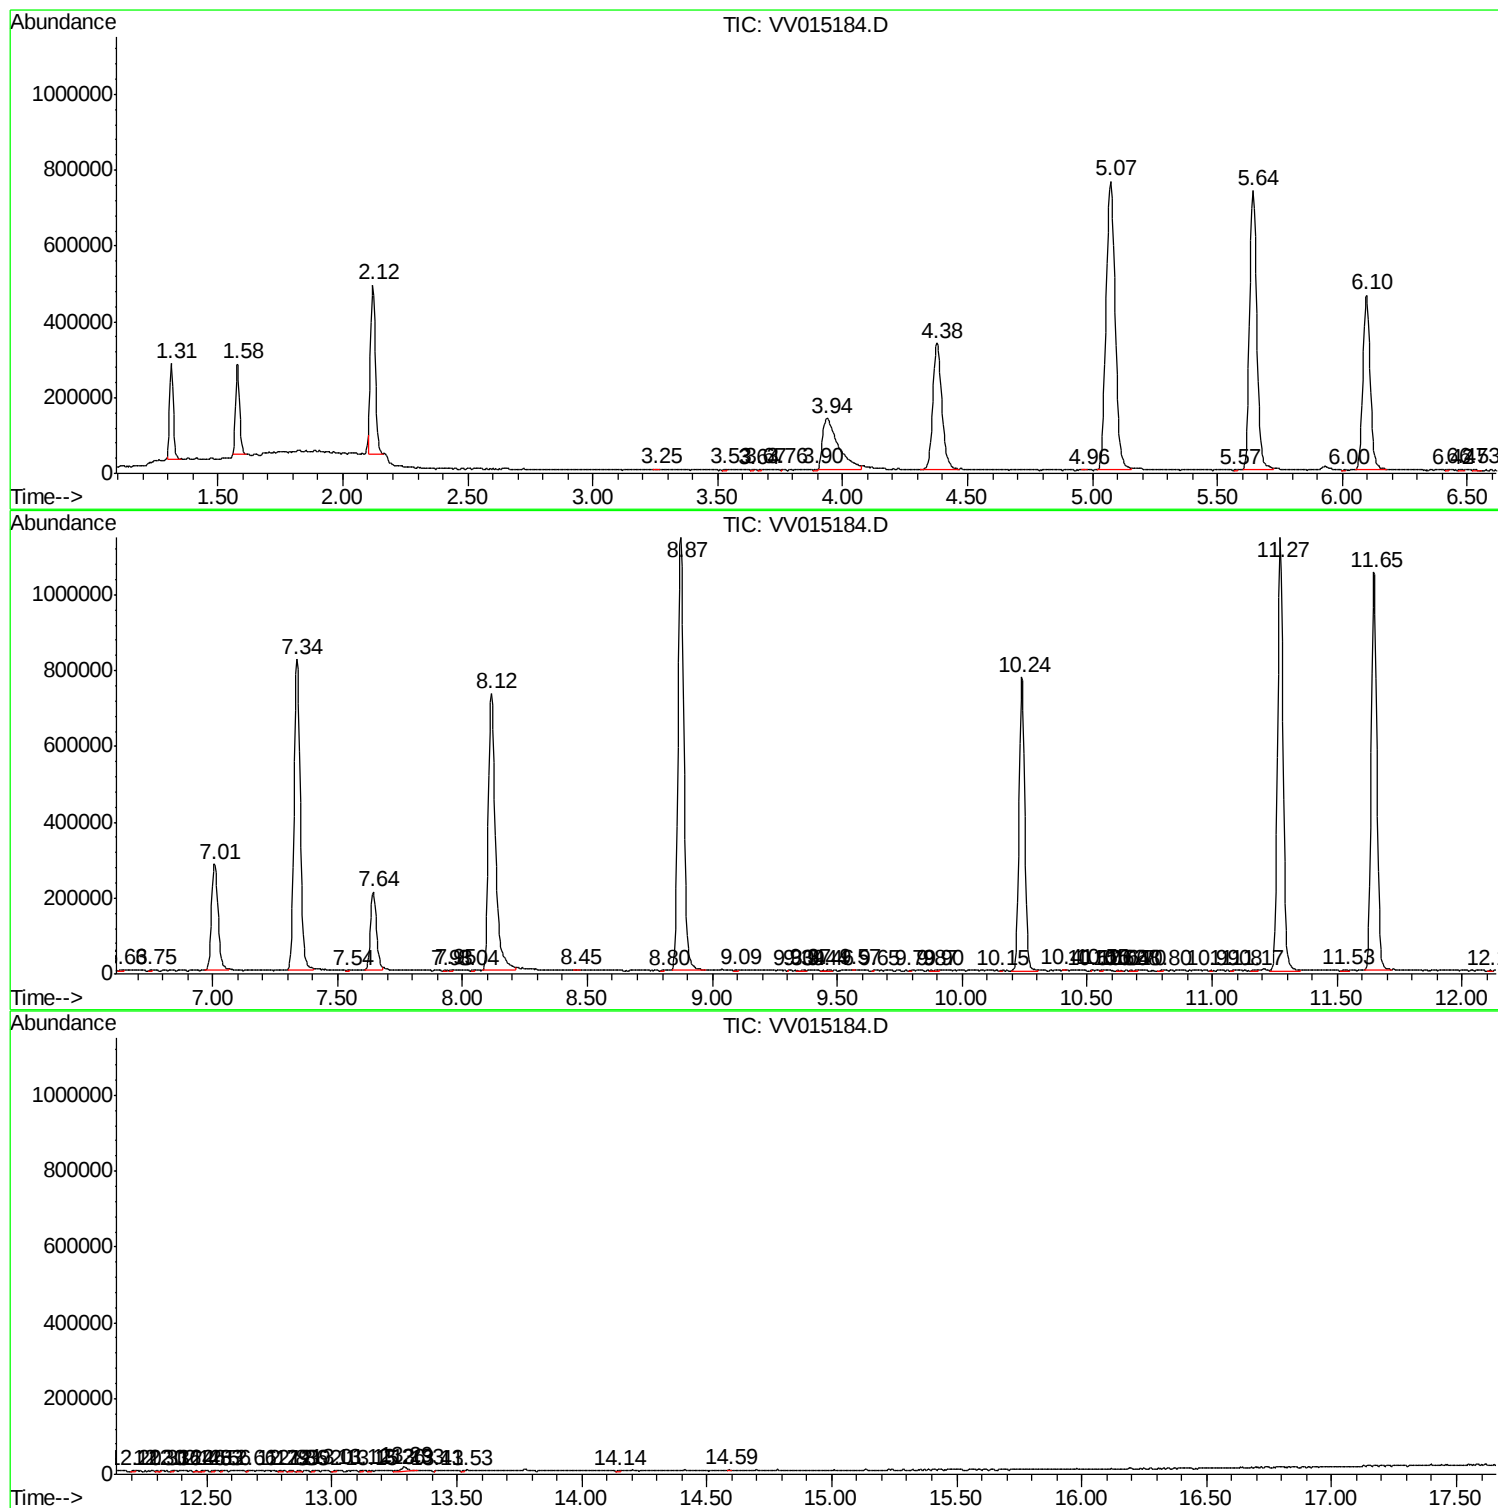

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015184.D
Acq On : 26 Mar 2020 23:01
Operator : SY/MD
Sample : VIBLK73
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK73

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015184.D
Acq On : 26 Mar 2020 23:01
Operator : SY/MD
Sample : VIBLK73
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK73

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc