

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015188.D
 Acq On : 27 Mar 2020 00:38
 Operator : SY/MD
 Sample : L1976-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	252814	247990	13.87%	1.546%
2	1.579	146	152	163	rBV	222187	260985	14.60%	1.627%
3	2.122	314	321	348	rVB	451339	720816	40.31%	4.494%
4	3.370	707	709	710	rBV2	1672	906	0.05%	0.006%
5	3.495	745	748	751	rVB4	2247	1436	0.08%	0.009%
6	3.515	751	754	760	rBV9	2618	3139	0.18%	0.020%
7	3.730	818	821	825	rBV6	2359	2140	0.12%	0.013%
8	3.753	825	828	832	rVV6	1725	1101	0.06%	0.007%
9	3.814	844	847	850	rBV5	1711	1467	0.08%	0.009%
10	3.859	856	861	863	rBV4	2154	1997	0.11%	0.012%
11	3.939	873	886	922	rBV	124736	489674	27.39%	3.053%
12	4.380	1009	1023	1050	rVB	296017	745374	41.69%	4.647%
13	4.698	1119	1122	1125	rVB5	2408	1585	0.09%	0.010%
14	4.801	1152	1154	1159	rBV6	2135	1580	0.09%	0.010%
15	4.826	1159	1162	1165	rVB5	3035	1926	0.11%	0.012%
16	4.849	1166	1169	1171	rBV4	1476	1049	0.06%	0.007%
17	5.074	1223	1239	1267	rVV2	709751	1788074	100.00%	11.148%
18	5.334	1318	1320	1326	rVB7	2268	2002	0.11%	0.012%
19	5.360	1326	1328	1329	rBV2	1807	929	0.05%	0.006%
20	5.402	1338	1341	1342	rBV3	1603	1134	0.06%	0.007%
21	5.473	1361	1363	1367	rBV4	2053	1331	0.07%	0.008%
22	5.563	1388	1391	1394	rBV5	2788	2345	0.13%	0.015%
23	5.643	1401	1416	1439	rBV	680614	1354746	75.77%	8.446%
24	5.939	1496	1508	1527	rBV	362481	694945	38.87%	4.333%
25	6.096	1545	1557	1577	rBV	415251	830931	46.47%	5.181%
26	6.315	1622	1625	1628	rBV4	1960	1526	0.09%	0.010%
27	6.360	1637	1639	1642	rBV3	1675	1056	0.06%	0.007%
28	6.392	1647	1649	1652	rBV3	2155	1615	0.09%	0.010%
29	6.444	1663	1665	1670	rBV6	1646	1415	0.08%	0.009%
30	6.543	1692	1696	1697	rBV4	1476	923	0.05%	0.006%
31	6.611	1714	1717	1720	rBV5	2202	1745	0.10%	0.011%
32	6.759	1758	1763	1766	rBV5	3246	2388	0.13%	0.015%
33	7.010	1830	1841	1860	rVV	177212	318612	17.82%	1.986%
34	7.113	1871	1873	1877	rBV4	1291	1070	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015188.D
 Acq On : 27 Mar 2020 00:38
 Operator : SY/MD
 Sample : L1976-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	7.215	1903	1905	1908	rVB4	1588	904	0.05%	0.006%
36	7.238	1908	1912	1914	rVB5	1797	1201	0.07%	0.007%
37	7.260	1914	1919	1921	rBV5	1983	1504	0.08%	0.009%
38	7.338	1929	1943	1963	rBV	829185	1444767	80.80%	9.008%
39	7.543	2004	2007	2009	rBV3	2351	1966	0.11%	0.012%
40	7.643	2027	2038	2053	rBV	127273	222567	12.45%	1.388%
41	7.891	2112	2115	2117	rBV4	1939	1100	0.06%	0.007%
42	7.958	2128	2136	2139	rBV9	4109	5471	0.31%	0.034%
43	8.116	2174	2185	2213	rBV2	559503	1146995	64.15%	7.151%
44	8.694	2359	2365	2368	rBV8	2321	2281	0.13%	0.014%
45	8.875	2409	2421	2442	rVV	1054373	1704513	95.33%	10.627%
46	9.029	2463	2469	2471	rBV6	2860	3441	0.19%	0.021%
47	9.122	2494	2498	2503	rBV8	3106	3082	0.17%	0.019%
48	9.257	2533	2540	2544	rBV8	2376	2706	0.15%	0.017%
49	9.280	2544	2547	2550	rBV5	2154	1554	0.09%	0.010%
50	9.360	2569	2572	2574	rBV4	1508	896	0.05%	0.006%
51	9.379	2574	2578	2580	rVV5	1611	1063	0.06%	0.007%
52	9.421	2588	2591	2593	rBV4	1447	985	0.06%	0.006%
53	9.479	2603	2609	2610	rBV5	1738	1864	0.10%	0.012%
54	9.585	2639	2642	2643	rBV3	1737	1033	0.06%	0.006%
55	9.646	2659	2661	2665	rVV6	2145	1416	0.08%	0.009%
56	9.710	2679	2681	2684	rBV4	1597	1145	0.06%	0.007%
57	9.948	2750	2755	2758	rBV6	1914	1919	0.11%	0.012%
58	9.987	2764	2767	2770	rBV5	3436	2381	0.13%	0.015%
59	10.058	2786	2789	2791	rBV4	2408	1824	0.10%	0.011%
60	10.100	2797	2802	2806	rBV8	2277	2350	0.13%	0.015%
61	10.238	2833	2845	2859	rBV	642375	1004364	56.17%	6.262%
62	10.447	2906	2910	2914	rBV5	2754	2160	0.12%	0.013%
63	10.495	2922	2925	2926	rBV3	1828	1118	0.06%	0.007%
64	10.518	2930	2932	2937	rBV5	1204	947	0.05%	0.006%
65	10.659	2974	2976	2977	rBV2	2100	989	0.06%	0.006%
66	10.762	3003	3008	3012	rVV7	1786	1871	0.10%	0.012%
67	10.865	3037	3040	3041	rBV3	2062	1095	0.06%	0.007%
68	11.083	3106	3108	3113	rBV6	2119	1234	0.07%	0.008%
69	11.196	3140	3143	3147	rBV6	2953	2275	0.13%	0.014%
70	11.270	3153	3166	3186	rBV	983682	1540893	86.18%	9.607%
71	11.514	3240	3242	3246	rBV4	1254	1090	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015188.D
 Acq On : 27 Mar 2020 00:38
 Operator : SY/MD
 Sample : L1976-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.563	3250	3257	3264	rBV7	6659	11800	0.66%	0.074%
73	11.649	3271	3284	3301	rBV	885044	1384568	77.43%	8.632%
74	11.849	3342	3346	3347	rBV4	1960	1320	0.07%	0.008%
75	11.907	3362	3364	3367	rBV4	2205	1397	0.08%	0.009%
76	12.064	3411	3413	3415	rBV3	1521	885	0.05%	0.006%
77	12.148	3436	3439	3441	rBV4	2084	1288	0.07%	0.008%
78	12.235	3464	3466	3471	rVB6	2038	1683	0.09%	0.010%
79	12.267	3471	3476	3477	rBV4	2214	1412	0.08%	0.009%
80	12.276	3477	3479	3483	rBV4	1689	1415	0.08%	0.009%
81	12.476	3537	3541	3546	rVB7	1970	1798	0.10%	0.011%
82	12.505	3546	3550	3553	rBV6	1943	1778	0.10%	0.011%
83	12.582	3572	3574	3579	rBV5	1705	1073	0.06%	0.007%
84	12.630	3587	3589	3593	rVB4	2571	1344	0.08%	0.008%
85	12.755	3625	3628	3630	rBV4	1848	1455	0.08%	0.009%
86	12.807	3642	3644	3646	rBV3	1931	992	0.06%	0.006%
87	12.900	3670	3673	3674	rBV4	1742	960	0.05%	0.006%
88	12.942	3682	3686	3690	rBV6	1664	1294	0.07%	0.008%
89	13.006	3703	3706	3708	rBV3	1552	885	0.05%	0.006%
90	13.064	3720	3724	3725	rBV3	1503	1093	0.06%	0.007%
91	13.167	3752	3756	3757	rBV4	1728	950	0.05%	0.006%
92	13.238	3775	3778	3783	rBV7	2200	1687	0.09%	0.011%
93	13.456	3843	3846	3849	rVB6	1796	1108	0.06%	0.007%
94	13.476	3849	3852	3854	rBV4	2103	1497	0.08%	0.009%
95	13.501	3858	3860	3863	rBV4	1829	1055	0.06%	0.007%
96	13.582	3882	3885	3887	rBV4	1507	937	0.05%	0.006%
97	13.984	4008	4010	4014	rVB4	2337	1117	0.06%	0.007%
98	14.292	4104	4106	4110	rBV5	1635	1306	0.07%	0.008%
99	14.443	4150	4153	4155	rBV4	1827	1339	0.07%	0.008%
100	14.524	4175	4178	4179	rBV3	2106	1133	0.06%	0.007%


Sum of corrected areas: 16039485

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015188.D
Acq On : 27 Mar 2020 00:38
Operator : SY/MD
Sample : L1976-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
ETTK8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

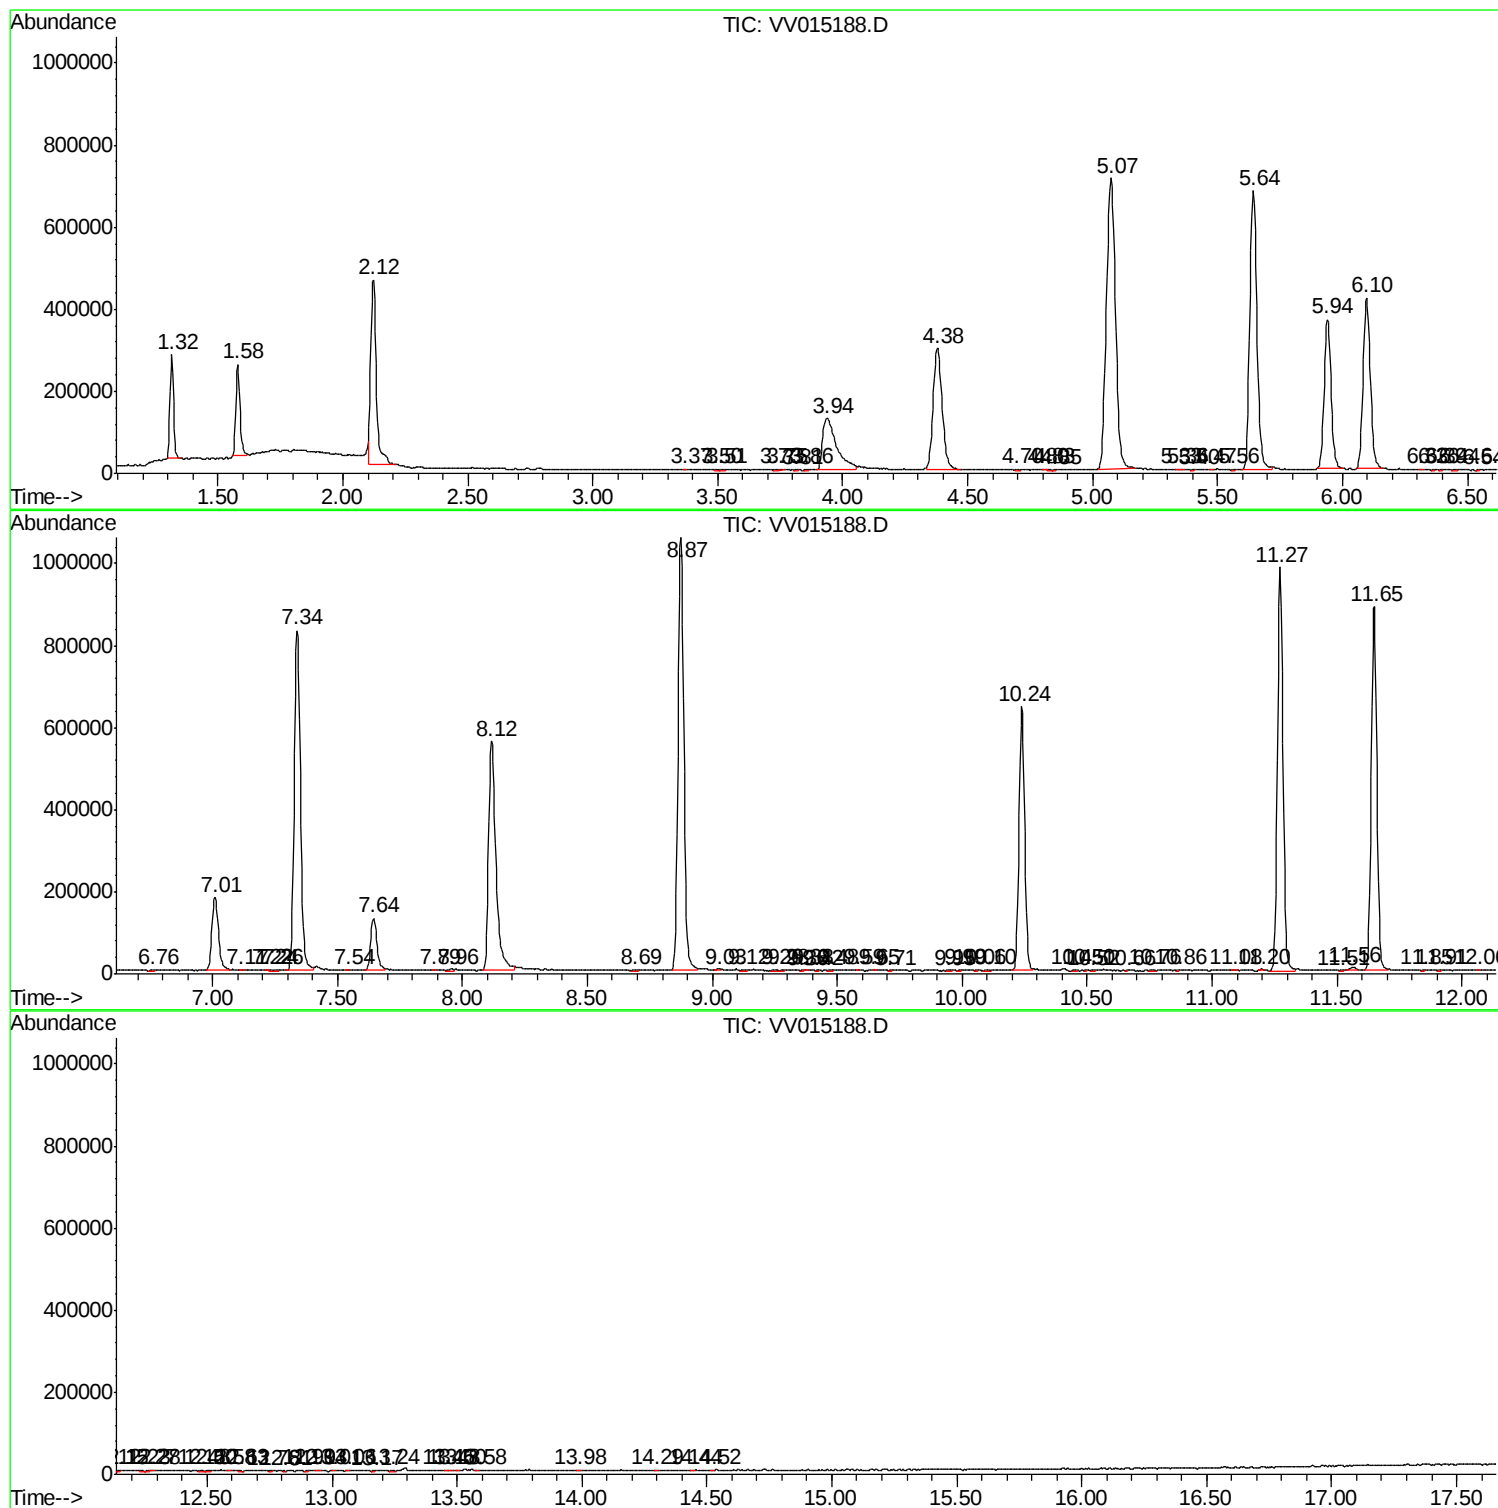

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015188.D
Acq On : 27 Mar 2020 00:38
Operator : SY/MD
Sample : L1976-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015188.D
Acq On : 27 Mar 2020 00:38
Operator : SY/MD
Sample : L1976-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc