

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015189.D
 Acq On : 27 Mar 2020 01:02
 Operator : SY/MD
 Sample : L1976-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	66	70	79	rVB	145052	135877	11.03%	1.500%
2	1.579	147	152	164	rVB	158256	177540	14.41%	1.960%
3	3.148	637	640	644	rBV4	2204	2160	0.18%	0.024%
4	3.363	705	707	709	rBV3	1684	935	0.08%	0.010%
5	3.605	779	782	785	rBV3	1582	1421	0.12%	0.016%
6	3.701	809	812	814	rBV4	2042	1234	0.10%	0.014%
7	3.878	863	867	870	rBV6	1814	1347	0.11%	0.015%
8	3.933	873	884	929	rBV	120784	517301	41.98%	5.710%
9	4.379	1009	1023	1043	rVB	217274	533337	43.28%	5.887%
10	4.653	1103	1108	1113	rBV8	2949	3700	0.30%	0.041%
11	4.752	1135	1139	1142	rBV5	2320	1904	0.15%	0.021%
12	4.859	1170	1172	1175	rBV4	1499	915	0.07%	0.010%
13	4.904	1184	1186	1188	rBV3	1363	816	0.07%	0.009%
14	5.071	1220	1238	1261	rBV2	473994	1232348	100.00%	13.604%
15	5.273	1299	1301	1303	rBV3	1362	674	0.05%	0.007%
16	5.537	1381	1383	1385	rBV3	2500	1463	0.12%	0.016%
17	5.643	1401	1416	1437	rBV	332115	678832	55.08%	7.493%
18	5.939	1496	1508	1525	rBV3	133165	272471	22.11%	3.008%
19	6.096	1544	1557	1579	rBV2	315358	650705	52.80%	7.183%
20	6.338	1630	1632	1634	rBV3	1470	710	0.06%	0.008%
21	6.428	1658	1660	1663	rVB3	1733	823	0.07%	0.009%
22	6.582	1703	1708	1712	rBV8	2665	3455	0.28%	0.038%
23	6.775	1766	1768	1770	rBV3	2023	1288	0.10%	0.014%
24	6.836	1782	1787	1788	rBV5	2101	2061	0.17%	0.023%
25	6.868	1794	1797	1799	rBV4	1940	1184	0.10%	0.013%
26	6.878	1799	1800	1804	rVV4	1801	693	0.06%	0.008%
27	6.971	1826	1829	1831	rBV4	2442	1964	0.16%	0.022%
28	7.010	1831	1841	1859	rVV2	127683	231112	18.75%	2.551%
29	7.257	1915	1918	1919	rBV3	1285	799	0.06%	0.009%
30	7.338	1933	1943	1961	rBV	324066	564232	45.79%	6.228%
31	7.569	2012	2015	2016	rBV3	1267	753	0.06%	0.008%
32	7.646	2030	2039	2054	rBV2	96182	159763	12.96%	1.764%
33	7.932	2125	2128	2130	rBV3	2134	1097	0.09%	0.012%
34	7.948	2131	2133	2135	rBV3	1651	761	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015189.D
 Acq On : 27 Mar 2020 01:02
 Operator : SY/MD
 Sample : L1976-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	8.045	2161	2163	2164	rBV	2626	1227	0.10%	0.014%
36	8.116	2174	2185	2220	rBV2	554221	1142005	92.67%	12.606%
37	8.421	2278	2280	2282	rVB3	1540	789	0.06%	0.009%
38	8.444	2283	2287	2290	rBV5	1906	1690	0.14%	0.019%
39	8.563	2320	2324	2326	rBV5	2357	1749	0.14%	0.019%
40	8.775	2386	2390	2393	rBV6	2093	1511	0.12%	0.017%
41	8.820	2400	2404	2408	rVB7	2168	1851	0.15%	0.020%
42	8.874	2409	2421	2440	rBV	424292	699443	56.76%	7.721%
43	9.247	2534	2537	2538	rBV3	1398	766	0.06%	0.008%
44	9.309	2549	2556	2558	rBV8	2520	2647	0.21%	0.029%
45	9.321	2558	2560	2565	rVB6	2383	1943	0.16%	0.021%
46	9.501	2611	2616	2619	rVB7	1881	1475	0.12%	0.016%
47	9.524	2619	2623	2624	rBV4	1328	1087	0.09%	0.012%
48	9.563	2630	2635	2638	rBV7	3083	3320	0.27%	0.037%
49	9.662	2662	2666	2668	rBV5	1936	1482	0.12%	0.016%
50	9.775	2697	2701	2705	rBV7	1887	1370	0.11%	0.015%
51	9.897	2737	2739	2742	rBV4	1519	839	0.07%	0.009%
52	10.051	2782	2787	2789	rBV5	1811	1457	0.12%	0.016%
53	10.238	2834	2845	2864	rBV	559388	875727	71.06%	9.667%
54	10.395	2892	2894	2897	rBV3	2284	1472	0.12%	0.016%
55	10.546	2936	2941	2944	rBV7	1893	1708	0.14%	0.019%
56	10.675	2978	2981	2982	rBV3	2493	1592	0.13%	0.018%
57	10.804	3017	3021	3023	rBV5	1801	1405	0.11%	0.016%
58	10.842	3031	3033	3035	rVV3	1909	1251	0.10%	0.014%
59	10.868	3039	3041	3044	rBV3	1378	888	0.07%	0.010%
60	10.903	3050	3052	3053	rBV2	1506	716	0.06%	0.008%
61	10.955	3065	3068	3071	rBV4	1840	1388	0.11%	0.015%
62	10.993	3078	3080	3083	rVB4	1507	828	0.07%	0.009%
63	11.013	3083	3086	3090	rVB3	2864	2070	0.17%	0.023%
64	11.032	3090	3092	3095	rVB4	1929	955	0.08%	0.011%
65	11.058	3097	3100	3102	rBV4	1283	836	0.07%	0.009%
66	11.170	3133	3135	3138	rVB4	1825	742	0.06%	0.008%
67	11.193	3138	3142	3144	rBV4	1976	1633	0.13%	0.018%
68	11.273	3155	3167	3192	rBV	308691	493718	40.06%	5.450%
69	11.415	3209	3211	3216	rBV5	1532	1075	0.09%	0.012%
70	11.498	3232	3237	3239	rBV6	2021	1723	0.14%	0.019%
71	11.521	3239	3244	3246	rBV5	1374	1166	0.09%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015189.D
 Acq On : 27 Mar 2020 01:02
 Operator : SY/MD
 Sample : L1976-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTK9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.649	3272	3284	3304	rBV	357795	568048	46.09%	6.271%
73	11.910	3362	3365	3366	rBV3	2066	1065	0.09%	0.012%
74	11.968	3381	3383	3386	rBV4	1404	895	0.07%	0.010%
75	12.009	3394	3396	3401	rVB6	1270	1046	0.08%	0.012%
76	12.038	3401	3405	3410	rBV6	2583	2793	0.23%	0.031%
77	12.090	3420	3421	3427	rVB5	2578	1762	0.14%	0.019%
78	12.119	3428	3430	3433	rBV3	1258	793	0.06%	0.009%
79	12.167	3442	3445	3448	rBV5	1624	1414	0.11%	0.016%
80	12.225	3459	3463	3466	rBV6	1825	1442	0.12%	0.016%
81	12.279	3478	3480	3486	rVB6	2326	2150	0.17%	0.024%
82	12.308	3486	3489	3492	rBV5	3408	1988	0.16%	0.022%
83	12.341	3496	3499	3503	rBV6	2148	2266	0.18%	0.025%
84	12.505	3547	3550	3551	rBV3	1379	764	0.06%	0.008%
85	12.614	3581	3584	3588	rBV5	1932	1793	0.15%	0.020%
86	12.636	3588	3591	3593	rVB4	2026	1162	0.09%	0.013%
87	12.649	3593	3595	3597	rBV3	1882	943	0.08%	0.010%
88	12.858	3656	3660	3663	rBV6	1749	1706	0.14%	0.019%
89	13.132	3743	3745	3747	rBV3	1730	762	0.06%	0.008%
90	13.292	3786	3795	3798	rBV10	5922	8282	0.67%	0.091%
91	13.514	3858	3864	3865	rBV6	2250	2161	0.18%	0.024%
92	13.636	3898	3902	3906	rBV6	2079	2071	0.17%	0.023%
93	13.717	3923	3927	3929	rBV5	2149	1933	0.16%	0.021%
94	13.871	3971	3975	3977	rBV5	1769	1450	0.12%	0.016%
95	13.903	3984	3985	3988	rBV3	1370	868	0.07%	0.010%
96	14.276	4097	4101	4103	rBV5	1760	1473	0.12%	0.016%
97	14.466	4158	4160	4163	rBV4	2406	1409	0.11%	0.016%
98	14.549	4184	4186	4189	rBV4	2531	1507	0.12%	0.017%
99	14.723	4238	4240	4241	rBV2	1895	923	0.07%	0.010%
100	15.180	4381	4382	4384	rBV2	1842	857	0.07%	0.009%


Sum of corrected areas: 9058945

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015189.D
Acq On : 27 Mar 2020 01:02
Operator : SY/MD
Sample : L1976-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
ETTK9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

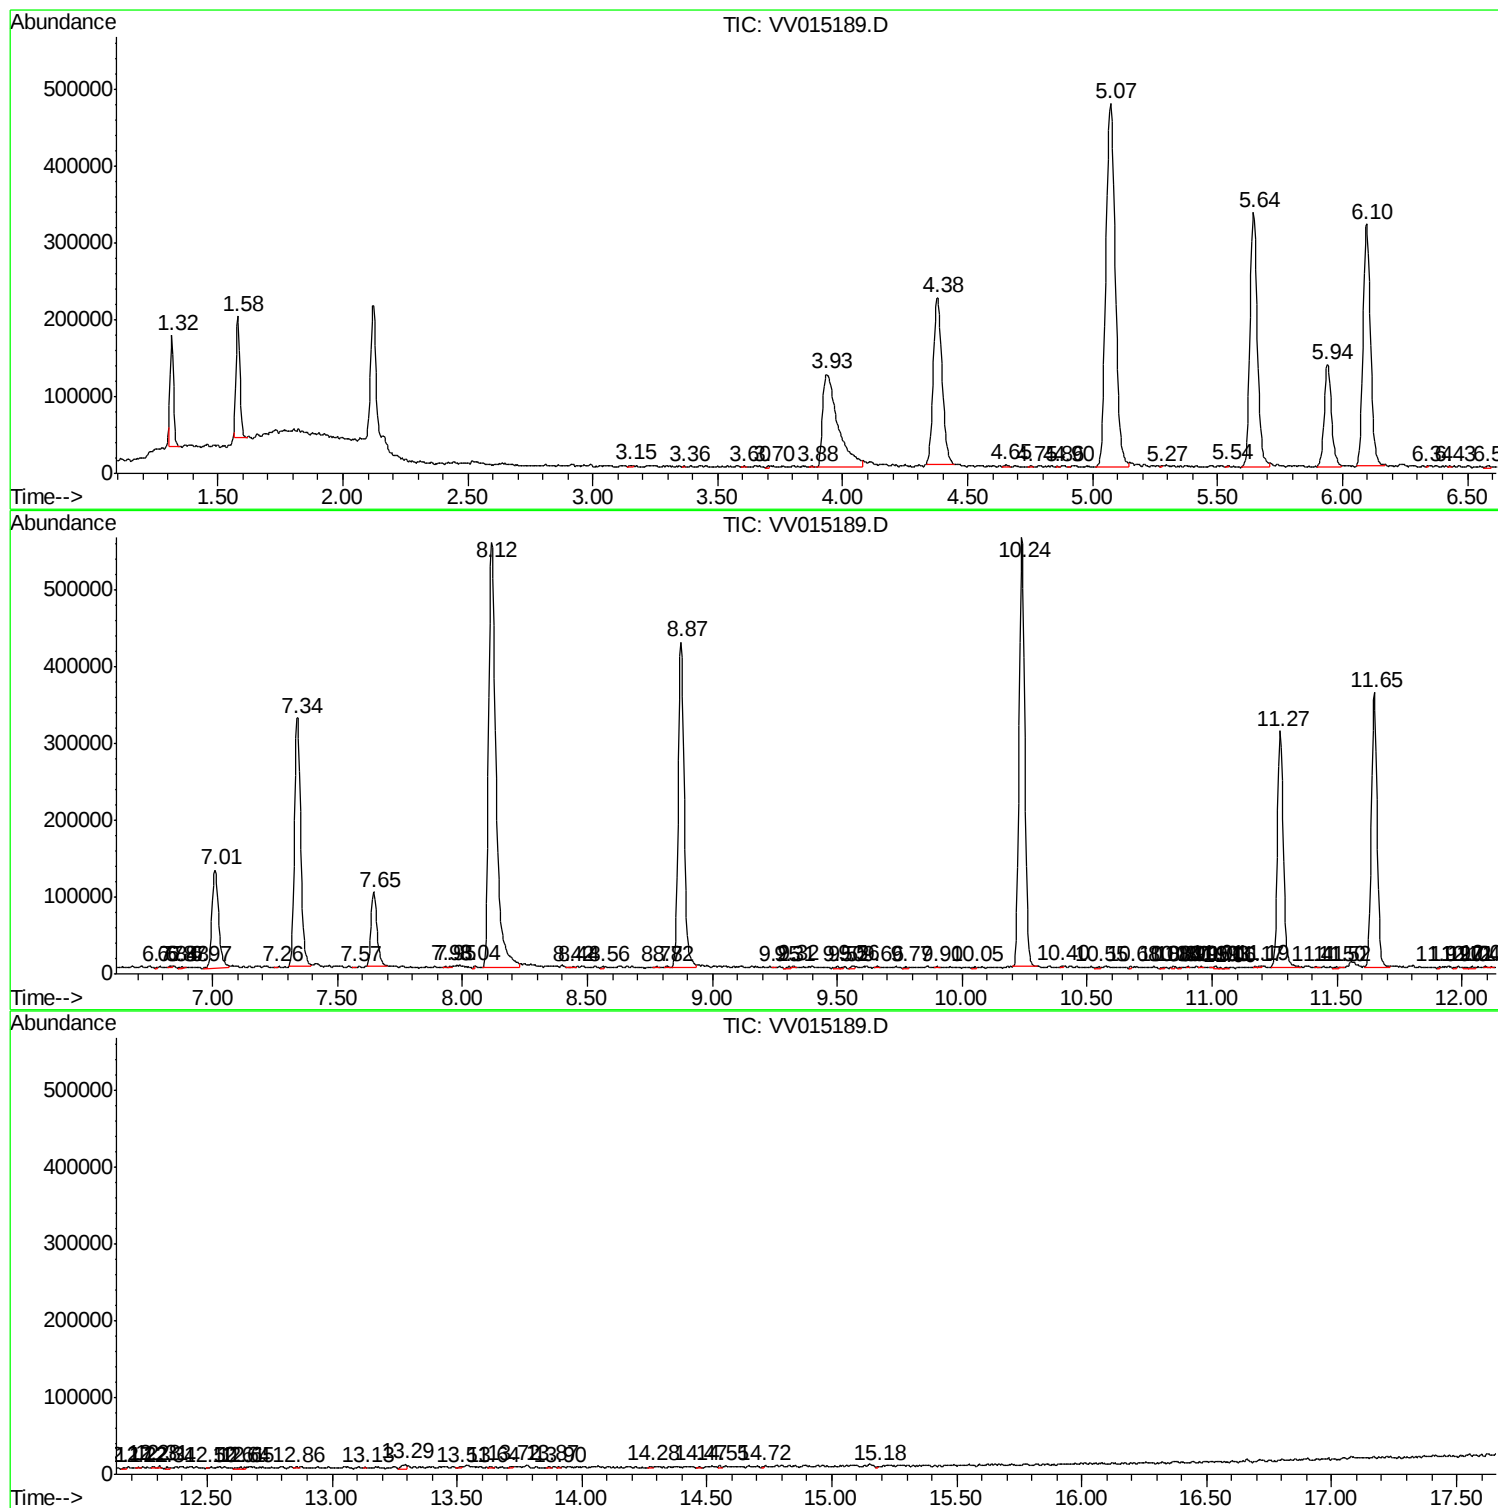

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015189.D
Acq On : 27 Mar 2020 01:02
Operator : SY/MD
Sample : L1976-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTK9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015189.D
Acq On : 27 Mar 2020 01:02
Operator : SY/MD
Sample : L1976-05
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTK9

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc