

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015190.D
 Acq On : 27 Mar 2020 01:26
 Operator : SY/MD
 Sample : L1976-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	83	rVB2	363174	393619	22.35%	2.598%
2	1.579	146	152	165	rVB	220603	260751	14.81%	1.721%
3	2.119	313	320	334	rVB	435696	622475	35.34%	4.108%
4	3.129	632	634	635	rBV2	1479	634	0.04%	0.004%
5	3.174	645	648	651	rBV5	2457	1851	0.11%	0.012%
6	3.454	733	735	740	rBV5	1666	1337	0.08%	0.009%
7	3.795	839	841	844	rBV2	1858	851	0.05%	0.006%
8	3.939	873	886	927	rBV	123158	534978	30.38%	3.531%
9	4.377	1010	1022	1046	rVB	295217	729695	41.43%	4.816%
10	4.727	1129	1131	1134	rBV4	1486	1136	0.06%	0.007%
11	4.788	1148	1150	1153	rBV4	2425	1354	0.08%	0.009%
12	5.074	1223	1239	1263	rBV2	704022	1761214	100.00%	11.624%
13	5.360	1325	1328	1330	rBV3	2204	1325	0.08%	0.009%
14	5.418	1340	1346	1350	rBV8	2066	2516	0.14%	0.017%
15	5.460	1356	1359	1360	rBV3	2060	1088	0.06%	0.007%
16	5.643	1403	1416	1441	rBV	664306	1317139	74.79%	8.693%
17	6.097	1544	1557	1579	rBV	418811	848936	48.20%	5.603%
18	6.286	1614	1616	1619	rBV4	1703	956	0.05%	0.006%
19	6.418	1655	1657	1659	rBV3	1712	853	0.05%	0.006%
20	6.441	1663	1664	1667	rBV3	1398	857	0.05%	0.006%
21	6.483	1675	1677	1679	rBV3	2244	1293	0.07%	0.009%
22	6.518	1685	1688	1692	rBV5	1606	1249	0.07%	0.008%
23	6.630	1721	1723	1725	rBV3	1187	692	0.04%	0.005%
24	6.643	1725	1727	1733	rVV7	2308	2115	0.12%	0.014%
25	6.753	1759	1761	1763	rBV3	1724	698	0.04%	0.005%
26	6.846	1786	1790	1792	rBV4	1797	1492	0.08%	0.010%
27	6.856	1792	1793	1795	rVV2	2229	753	0.04%	0.005%
28	6.872	1796	1798	1802	rVB5	1909	984	0.06%	0.006%
29	7.010	1830	1841	1865	rBV	174406	318471	18.08%	2.102%
30	7.212	1901	1904	1905	rBV3	2018	1131	0.06%	0.007%
31	7.338	1931	1943	1963	rBV	816732	1409181	80.01%	9.301%
32	7.576	2010	2017	2020	rBV8	2278	2478	0.14%	0.016%
33	7.592	2020	2022	2026	rVB5	1866	1151	0.07%	0.008%
34	7.643	2026	2038	2057	rBV	126054	227672	12.93%	1.503%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015190.D
 Acq On : 27 Mar 2020 01:26
 Operator : SY/MD
 Sample : L1976-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	8.116	2175	2185	2220	rBV2	549568	1139682	64.71%	7.522%
36	8.405	2273	2275	2279	rBV4	1915	1265	0.07%	0.008%
37	8.476	2291	2297	2300	rBV6	2519	2868	0.16%	0.019%
38	8.605	2335	2337	2343	rBV6	1957	1768	0.10%	0.012%
39	8.653	2348	2352	2353	rBV3	1934	1169	0.07%	0.008%
40	8.788	2392	2394	2397	rVB4	1654	900	0.05%	0.006%
41	8.875	2408	2421	2444	rBV	1028374	1658141	94.15%	10.944%
42	9.161	2508	2510	2513	rBV4	1562	980	0.06%	0.006%
43	9.244	2534	2536	2544	rBV7	2220	2265	0.13%	0.015%
44	9.396	2578	2583	2585	rBV6	2580	2297	0.13%	0.015%
45	9.495	2611	2614	2616	rBV4	1922	1291	0.07%	0.009%
46	9.534	2624	2626	2628	rBV2	1468	572	0.03%	0.004%
47	9.569	2632	2637	2639	rBV6	2316	1836	0.10%	0.012%
48	9.717	2681	2683	2685	rBV3	1471	765	0.04%	0.005%
49	9.765	2695	2698	2700	rBV4	1861	1274	0.07%	0.008%
50	9.817	2712	2714	2717	rVB3	1685	964	0.05%	0.006%
51	9.833	2717	2719	2720	rBV2	1274	568	0.03%	0.004%
52	9.884	2733	2735	2736	rBV2	1157	504	0.03%	0.003%
53	9.897	2736	2739	2742	rVV6	2914	2076	0.12%	0.014%
54	10.003	2770	2772	2774	rBV3	1480	635	0.04%	0.004%
55	10.042	2780	2784	2789	rBV6	3253	2717	0.15%	0.018%
56	10.064	2789	2791	2794	rVB4	1908	854	0.05%	0.006%
57	10.122	2806	2809	2812	rBV5	2169	1338	0.08%	0.009%
58	10.238	2834	2845	2866	rVB	632145	998944	56.72%	6.593%
59	10.379	2887	2889	2892	rBV3	1904	1132	0.06%	0.007%
60	10.444	2907	2909	2910	rBV	1720	767	0.04%	0.005%
61	10.463	2914	2915	2918	rVB3	1813	892	0.05%	0.006%
62	10.479	2918	2920	2923	rBV4	1839	1396	0.08%	0.009%
63	10.527	2932	2935	2939	rBV6	1755	1360	0.08%	0.009%
64	10.611	2957	2961	2962	rBV4	1490	997	0.06%	0.007%
65	10.707	2989	2991	2992	rBV2	1675	758	0.04%	0.005%
66	10.916	3054	3056	3060	rBV4	1299	1317	0.07%	0.009%
67	11.164	3129	3133	3135	rBV5	1878	1551	0.09%	0.010%
68	11.270	3155	3166	3185	rBV	932725	1447068	82.16%	9.551%
69	11.466	3224	3227	3229	rBV4	2091	1177	0.07%	0.008%
70	11.524	3241	3245	3247	rBV4	1910	1285	0.07%	0.008%
71	11.563	3249	3257	3269	rVB2	11747	22463	1.28%	0.148%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015190.D
 Acq On : 27 Mar 2020 01:26
 Operator : SY/MD
 Sample : L1976-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.650	3270	3284	3301	rBV	850867	1354261	76.89%	8.938%
73	11.785	3324	3326	3327	rBV2	1270	565	0.03%	0.004%
74	11.875	3351	3354	3357	rBV4	2233	1313	0.07%	0.009%
75	11.987	3387	3389	3391	rBV3	1115	546	0.03%	0.004%
76	12.010	3394	3396	3397	rBV2	1716	549	0.03%	0.004%
77	12.032	3401	3403	3405	rBV3	1490	623	0.04%	0.004%
78	12.106	3424	3426	3434	rVB8	2207	2228	0.13%	0.015%
79	12.145	3434	3438	3441	rBV5	1763	1312	0.07%	0.009%
80	12.209	3454	3458	3462	rBV6	1780	1819	0.10%	0.012%
81	12.238	3464	3467	3469	rBV3	1960	1268	0.07%	0.008%
82	12.463	3535	3537	3542	rBV5	1541	1306	0.07%	0.009%
83	12.495	3543	3547	3549	rBV4	2374	1508	0.09%	0.010%
84	12.669	3596	3601	3602	rBV5	2103	1720	0.10%	0.011%
85	12.727	3616	3619	3625	rBV8	2148	1941	0.11%	0.013%
86	12.820	3643	3648	3652	rBV7	2512	2338	0.13%	0.015%
87	12.891	3665	3670	3671	rBV5	1585	1306	0.07%	0.009%
88	12.916	3676	3678	3680	rVB3	1768	783	0.04%	0.005%
89	12.952	3686	3689	3691	rBV3	1343	697	0.04%	0.005%
90	12.968	3691	3694	3697	rBV4	1615	1219	0.07%	0.008%
91	13.167	3753	3756	3758	rBV4	1345	887	0.05%	0.006%
92	13.260	3783	3785	3786	rBV3	2040	869	0.05%	0.006%
93	13.431	3835	3838	3841	rVB4	1930	1168	0.07%	0.008%
94	13.447	3841	3843	3845	rBV3	1615	712	0.04%	0.005%
95	13.858	3970	3971	3974	rVB3	2586	887	0.05%	0.006%
96	13.875	3974	3976	3977	rBV2	1415	513	0.03%	0.003%
97	14.161	4062	4065	4071	rBV8	3273	3521	0.20%	0.023%
98	14.379	4130	4133	4136	rBV4	2380	1362	0.08%	0.009%
99	14.405	4139	4141	4142	rBV2	1667	643	0.04%	0.004%
100	14.891	4289	4292	4294	rBV4	3803	2741	0.16%	0.018%


Sum of corrected areas: 15151366

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015190.D
Acq On : 27 Mar 2020 01:26
Operator : SY/MD
Sample : L1976-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
ETTL1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

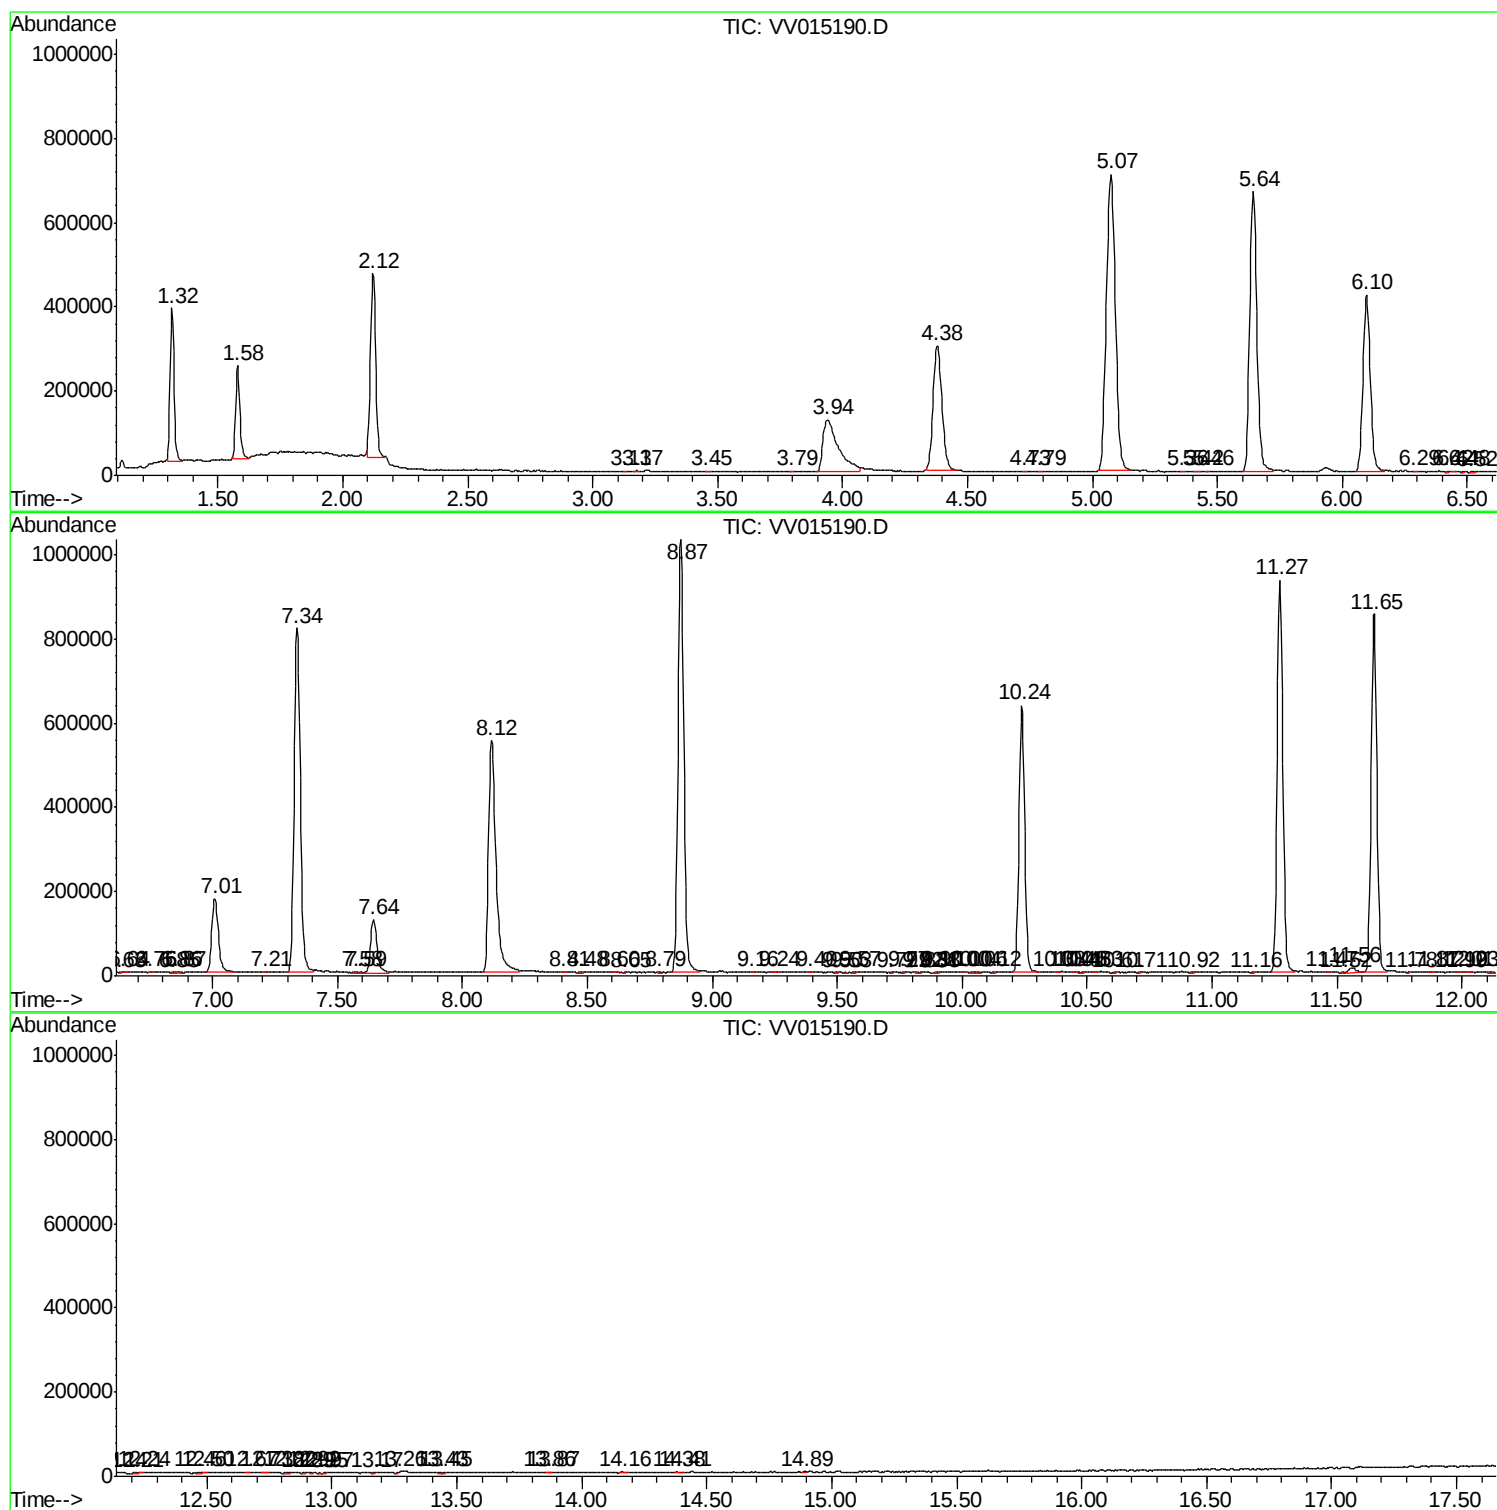

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015190.D
Acq On : 27 Mar 2020 01:26
Operator : SY/MD
Sample : L1976-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015190.D
Acq On : 27 Mar 2020 01:26
Operator : SY/MD
Sample : L1976-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc