

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015191.D
 Acq On : 27 Mar 2020 01:51
 Operator : SY/MD
 Sample : L1976-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	78	rVB	235741	238723	2.86%	1.044%
2	1.579	146	152	163	rBV	222307	256484	3.08%	1.121%
3	2.123	314	321	348	rVB	449382	721129	8.65%	3.153%
4	2.779	518	525	540	rVB	55436	94677	1.14%	0.414%
5	3.061	610	613	615	rBV3	1735	980	0.01%	0.004%
6	3.119	628	631	633	rBV4	2500	1574	0.02%	0.007%
7	3.151	639	641	643	rBV3	1829	826	0.01%	0.004%
8	3.306	688	689	692	rBV3	1231	568	0.01%	0.002%
9	3.335	696	698	699	rBV2	1598	847	0.01%	0.004%
10	3.537	760	761	765	rBV4	959	664	0.01%	0.003%
11	3.560	765	768	770	rVB4	2542	1417	0.02%	0.006%
12	3.627	788	789	791	rBV2	666	212	0.00%	0.001%
13	3.643	791	794	797	rBV5	1782	1555	0.02%	0.007%
14	3.656	797	798	801	rVB3	2671	1066	0.01%	0.005%
15	3.676	801	804	805	rBV3	1507	774	0.01%	0.003%
16	3.730	818	821	822	rBV3	1498	777	0.01%	0.003%
17	3.788	836	839	842	rBV4	1856	1292	0.02%	0.006%
18	3.939	870	886	923	rBV	3412394	8333887	100.00%	36.437%
19	4.380	1009	1023	1046	rVB	294177	724080	8.69%	3.166%
20	4.843	1165	1167	1169	rBV3	1225	548	0.01%	0.002%
21	4.920	1187	1191	1192	rBV3	1451	898	0.01%	0.004%
22	4.949	1197	1200	1201	rBV3	2142	999	0.01%	0.004%
23	5.074	1218	1239	1266	rBV2	702651	1773692	21.28%	7.755%
24	5.483	1363	1366	1369	rBV5	1533	1293	0.02%	0.006%
25	5.643	1402	1416	1438	rBV	661233	1330601	15.97%	5.818%
26	6.097	1544	1557	1579	rBV	418385	835595	10.03%	3.653%
27	6.293	1615	1618	1621	rBV4	1982	1807	0.02%	0.008%
28	6.367	1638	1641	1643	rBV3	2394	1508	0.02%	0.007%
29	6.444	1661	1665	1667	rBV6	2893	2001	0.02%	0.009%
30	6.560	1699	1701	1702	rBV3	581	267	0.00%	0.001%
31	6.608	1711	1716	1717	rBV5	1149	926	0.01%	0.004%
32	6.634	1721	1724	1727	rBV4	1557	766	0.01%	0.003%
33	6.650	1727	1729	1732	rBV3	2187	1374	0.02%	0.006%
34	6.746	1757	1759	1761	rBV3	902	393	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015191.D
 Acq On : 27 Mar 2020 01:51
 Operator : SY/MD
 Sample : L1976-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	6.762	1761	1764	1765	rBV3	1370	652	0.01%	0.003%
36	6.798	1772	1775	1776	rBV3	1471	785	0.01%	0.003%
37	6.833	1782	1786	1789	rBV5	1482	1361	0.02%	0.006%
38	6.910	1808	1810	1811	rBV2	954	376	0.00%	0.002%
39	6.933	1816	1817	1819	rBV2	1196	540	0.01%	0.002%
40	6.968	1826	1828	1830	rBV3	1403	607	0.01%	0.003%
41	7.010	1830	1841	1859	rBV	169698	311614	3.74%	1.362%
42	7.209	1900	1903	1906	rBV4	1765	1484	0.02%	0.006%
43	7.338	1931	1943	1963	rBV	805675	1380220	16.56%	6.034%
44	7.643	2029	2038	2057	rBV	122462	209378	2.51%	0.915%
45	7.913	2118	2122	2125	rBV4	2323	1822	0.02%	0.008%
46	7.962	2134	2137	2139	rBV3	2024	1199	0.01%	0.005%
47	8.000	2145	2149	2153	rBV6	1538	1170	0.01%	0.005%
48	8.071	2169	2171	2174	rBV4	992	663	0.01%	0.003%
49	8.116	2174	2185	2211	rBV3	566686	1150858	13.81%	5.032%
50	8.447	2286	2288	2293	rBV6	1987	1281	0.02%	0.006%
51	8.585	2328	2331	2333	rBV4	1796	987	0.01%	0.004%
52	8.704	2363	2368	2371	rBV6	1651	1980	0.02%	0.009%
53	8.736	2375	2378	2381	rBV5	1152	764	0.01%	0.003%
54	8.753	2381	2383	2386	rBV3	1300	759	0.01%	0.003%
55	8.875	2409	2421	2445	rBV	1022677	1653135	19.84%	7.228%
56	9.100	2489	2491	2493	rBV3	1246	460	0.01%	0.002%
57	9.347	2560	2568	2570	rBV7	3094	3810	0.05%	0.017%
58	9.370	2573	2575	2578	rBV4	1023	562	0.01%	0.002%
59	9.630	2654	2656	2661	rBV5	2445	2430	0.03%	0.011%
60	9.769	2696	2699	2700	rBV4	1823	1040	0.01%	0.005%
61	9.913	2743	2744	2746	rBV2	1084	570	0.01%	0.002%
62	10.023	2776	2778	2782	rBV4	2253	1260	0.02%	0.006%
63	10.148	2807	2817	2824	rBV4	4136	8398	0.10%	0.037%
64	10.177	2824	2826	2829	rBV5	1286	959	0.01%	0.004%
65	10.238	2834	2845	2862	rVB	638254	992832	11.91%	4.341%
66	10.392	2888	2893	2894	rBV5	2664	2094	0.03%	0.009%
67	10.560	2942	2945	2946	rBV3	1845	870	0.01%	0.004%
68	10.733	2992	2999	3000	rBV7	2787	2462	0.03%	0.011%
69	11.077	3098	3106	3108	rBV8	6940	8491	0.10%	0.037%
70	11.170	3131	3135	3137	rBV4	2131	1874	0.02%	0.008%
71	11.270	3155	3166	3191	rBV	932320	1440728	17.29%	6.299%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015191.D
 Acq On : 27 Mar 2020 01:51
 Operator : SY/MD
 Sample : L1976-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTL4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.534	3244	3248	3249	rBV3	2725	1766	0.02%	0.008%
73	11.560	3249	3256	3263	rVV8	6891	12721	0.15%	0.056%
74	11.646	3272	3283	3300	rBV	809935	1280047	15.36%	5.597%
75	11.920	3364	3368	3369	rBV3	1712	1300	0.02%	0.006%
76	12.129	3431	3433	3435	rBV3	1826	1059	0.01%	0.005%
77	12.257	3470	3473	3474	rBV3	4638	2981	0.04%	0.013%
78	12.489	3540	3545	3553	rVB4	13000	18785	0.23%	0.082%
79	12.569	3568	3570	3578	rVB8	3430	4175	0.05%	0.018%
80	12.617	3583	3585	3587	rBV3	1745	1052	0.01%	0.005%
81	12.630	3587	3589	3592	rVB3	2960	1573	0.02%	0.007%
82	12.662	3592	3599	3605	rBV9	6552	10422	0.13%	0.046%
83	12.749	3621	3626	3628	rBV6	1480	1246	0.01%	0.005%
84	12.836	3650	3653	3658	rBV7	2626	2921	0.04%	0.013%
85	12.952	3687	3689	3694	rBV6	3349	2167	0.03%	0.009%
86	13.254	3781	3783	3784	rBV2	2054	761	0.01%	0.003%
87	13.408	3829	3831	3832	rBV3	1552	634	0.01%	0.003%
88	13.601	3888	3891	3893	rBV4	1971	893	0.01%	0.004%
89	13.730	3929	3931	3934	rBV4	1883	1242	0.01%	0.005%
90	14.019	4019	4021	4023	rBV3	1352	945	0.01%	0.004%
91	14.736	4242	4244	4246	rBV3	1401	789	0.01%	0.003%


Sum of corrected areas: 22872154

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015191.D
Acq On : 27 Mar 2020 01:51
Operator : SY/MD
Sample : L1976-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

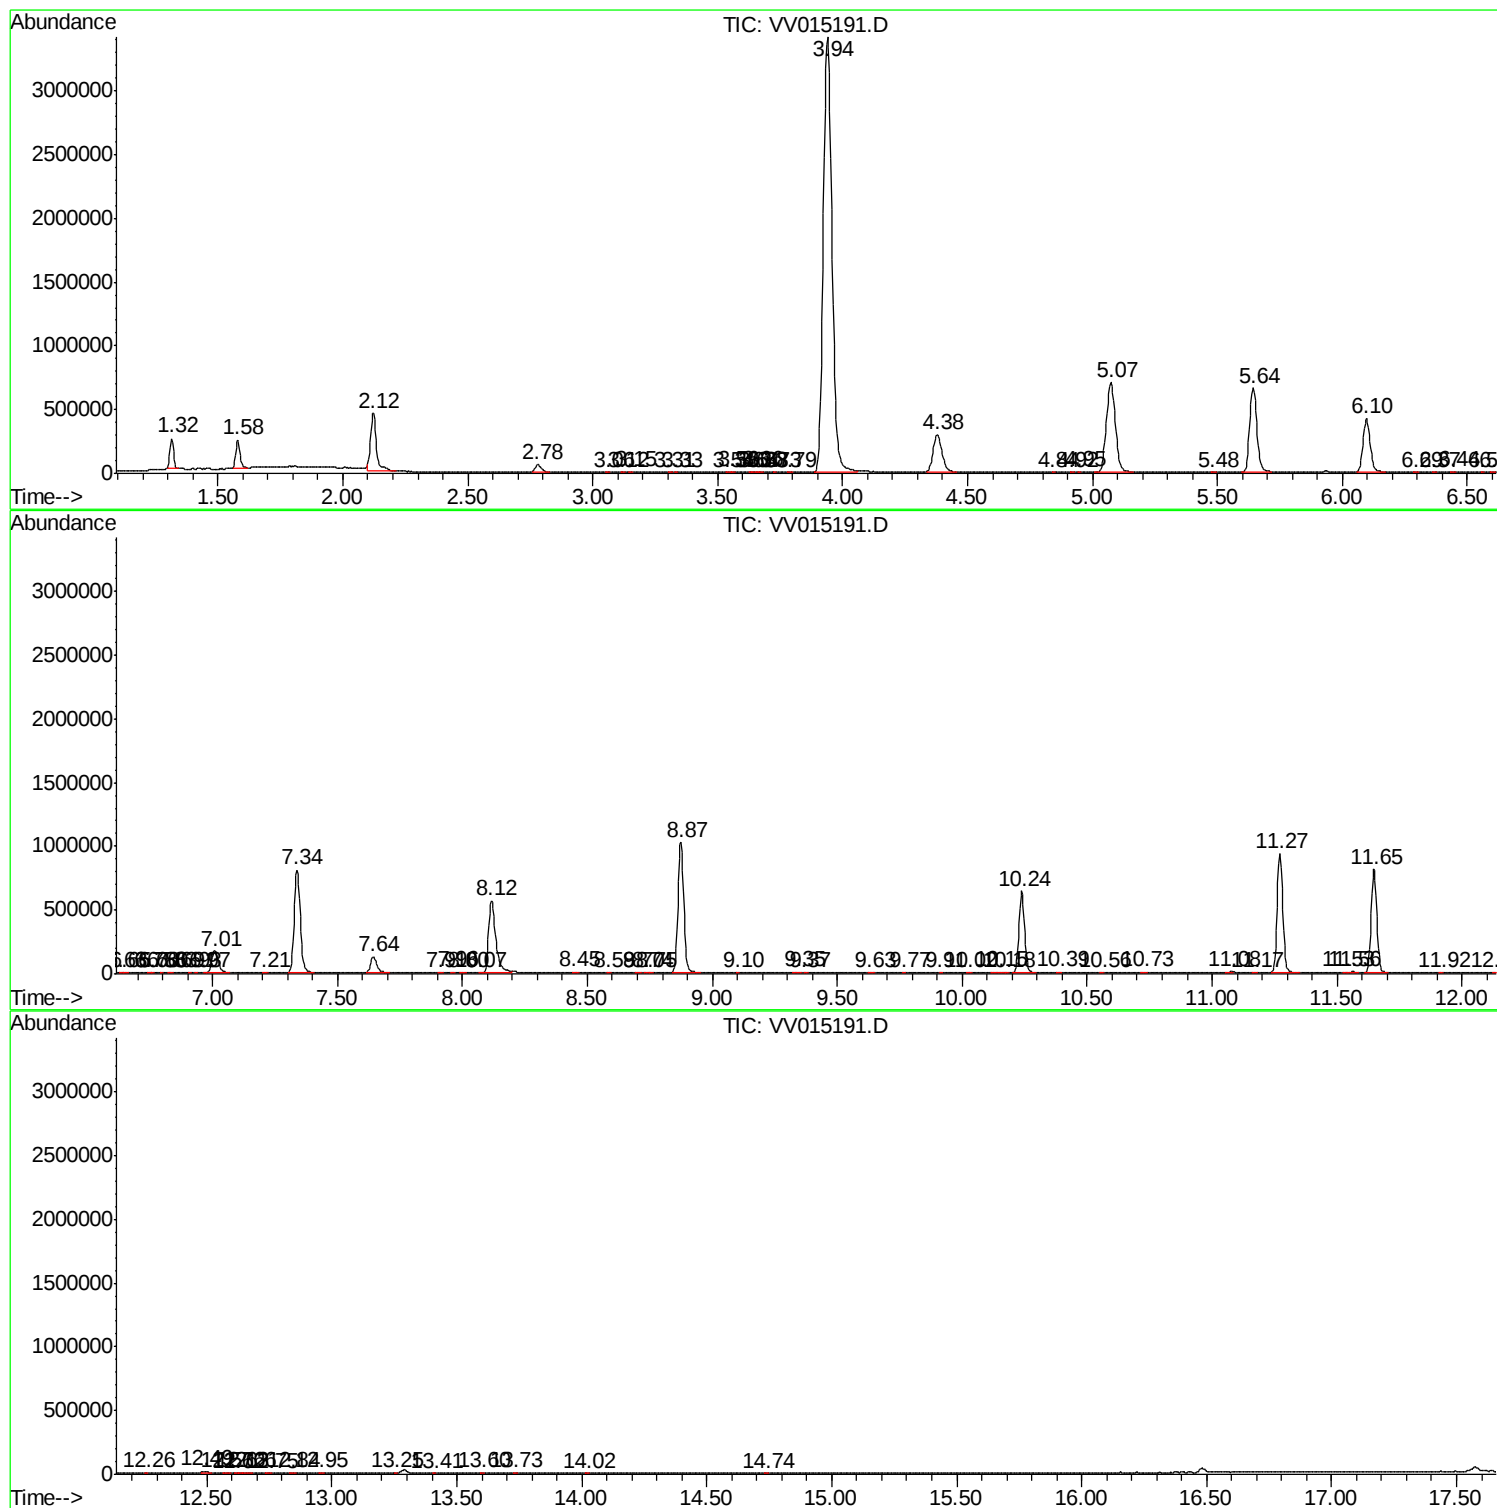

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015191.D
Acq On : 27 Mar 2020 01:51
Operator : SY/MD
Sample : L1976-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015191.D
Acq On : 27 Mar 2020 01:51
Operator : SY/MD
Sample : L1976-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTL4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc