

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015194.D
 Acq On : 27 Mar 2020 04:16
 Operator : SY/MD
 Sample : VV0326WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	249375	260745	13.64%	1.675%
2	1.579	146	152	166	rVB	219226	258258	13.51%	1.659%
3	2.119	313	320	332	rVB	485548	678818	35.51%	4.361%
4	3.045	605	608	609	rBV3	1467	886	0.05%	0.006%
5	3.177	645	649	651	rBV4	2779	2021	0.11%	0.013%
6	3.299	685	687	688	rBV2	2093	924	0.05%	0.006%
7	3.357	703	705	706	rBV3	1476	574	0.03%	0.004%
8	3.399	715	718	720	rBV4	2061	1219	0.06%	0.008%
9	3.682	800	806	808	rBV6	2562	2410	0.13%	0.015%
10	3.804	840	844	845	rBV4	1998	1249	0.07%	0.008%
11	3.830	850	852	854	rVB3	1576	622	0.03%	0.004%
12	3.859	857	861	864	rBV5	2950	2702	0.14%	0.017%
13	3.946	874	888	925	rBV2	95707	440894	23.06%	2.832%
14	4.380	1010	1023	1045	rVB	284064	693475	36.28%	4.455%
15	4.994	1211	1214	1219	rBV7	2164	1598	0.08%	0.010%
16	5.074	1223	1239	1264	rVV2	678215	1686251	88.21%	10.833%
17	5.380	1328	1334	1340	rBV10	2111	3142	0.16%	0.020%
18	5.544	1382	1385	1388	rBV5	2044	1351	0.07%	0.009%
19	5.560	1388	1390	1393	rBV4	2331	1758	0.09%	0.011%
20	5.643	1403	1416	1440	rBV	764854	1523459	79.69%	9.787%
21	5.984	1519	1522	1523	rBV3	1127	462	0.02%	0.003%
22	6.097	1544	1557	1580	rBV2	392223	797649	41.72%	5.124%
23	6.351	1630	1636	1638	rBV6	2002	2241	0.12%	0.014%
24	6.521	1685	1689	1691	rBV5	1450	1061	0.06%	0.007%
25	6.540	1691	1695	1699	rVV5	2100	2244	0.12%	0.014%
26	6.640	1721	1726	1730	rBV7	1806	2066	0.11%	0.013%
27	6.810	1777	1779	1783	rBV5	1673	818	0.04%	0.005%
28	6.900	1805	1807	1809	rBV3	1219	585	0.03%	0.004%
29	7.010	1827	1841	1858	rBV	239067	427781	22.38%	2.748%
30	7.199	1896	1900	1902	rBV4	1714	1319	0.07%	0.008%
31	7.235	1907	1911	1918	rBV9	2591	3062	0.16%	0.020%
32	7.338	1931	1943	1966	rBV	798074	1373049	71.82%	8.821%
33	7.643	2029	2038	2059	rBV	164777	280167	14.66%	1.800%
34	7.801	2084	2087	2093	rBV7	1948	1703	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015194.D
 Acq On : 27 Mar 2020 04:16
 Operator : SY/MD
 Sample : VV0326WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK94

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	7.836	2095	2098	2100	rBV4	1945	1046	0.05%	0.007%
36	7.945	2130	2132	2135	rBV4	2195	991	0.05%	0.006%
37	8.058	2164	2167	2171	rBV5	2197	1353	0.07%	0.009%
38	8.116	2175	2185	2223	rVV	495843	1024998	53.62%	6.585%
39	8.662	2351	2355	2357	rBV5	1331	1205	0.06%	0.008%
40	8.817	2401	2403	2405	rVB3	1620	642	0.03%	0.004%
41	8.875	2409	2421	2442	rVV	1175861	1911699	100.00%	12.281%
42	9.113	2491	2495	2498	rVB6	2185	1707	0.09%	0.011%
43	9.132	2498	2501	2503	rBV3	1414	842	0.04%	0.005%
44	9.164	2507	2511	2513	rBV4	2965	2778	0.15%	0.018%
45	9.199	2520	2522	2525	rBV4	1269	606	0.03%	0.004%
46	9.277	2542	2546	2549	rBV6	1448	1267	0.07%	0.008%
47	9.360	2569	2572	2577	rVB5	1452	865	0.05%	0.006%
48	9.383	2577	2579	2582	rBV3	1364	751	0.04%	0.005%
49	9.421	2588	2591	2592	rBV3	2360	1378	0.07%	0.009%
50	9.463	2599	2604	2606	rBV5	1937	1597	0.08%	0.010%
51	9.643	2657	2660	2664	rBV5	1528	1414	0.07%	0.009%
52	9.759	2695	2696	2700	rVB4	1551	866	0.05%	0.006%
53	9.817	2712	2714	2716	rVB3	1114	465	0.02%	0.003%
54	9.833	2716	2719	2724	rBV7	1622	1469	0.08%	0.009%
55	9.868	2728	2730	2733	rBV4	1552	883	0.05%	0.006%
56	9.942	2751	2753	2754	rBV2	2168	814	0.04%	0.005%
57	10.022	2775	2778	2781	rVV4	1468	1133	0.06%	0.007%
58	10.096	2793	2801	2805	rBV4	2052	3246	0.17%	0.021%
59	10.161	2819	2821	2825	rVB5	1856	1156	0.06%	0.007%
60	10.180	2825	2827	2829	rBV3	1501	797	0.04%	0.005%
61	10.238	2829	2845	2859	rBV	583337	926283	48.45%	5.950%
62	10.672	2978	2980	2982	rVB3	1840	755	0.04%	0.005%
63	10.688	2982	2985	2986	rBV3	2324	1333	0.07%	0.009%
64	10.727	2993	2997	2998	rBV4	1236	807	0.04%	0.005%
65	10.772	3009	3011	3014	rVB3	1918	840	0.04%	0.005%
66	10.784	3014	3015	3020	rBV4	1088	553	0.03%	0.004%
67	10.939	3053	3063	3067	rBV4	4491	7398	0.39%	0.048%
68	10.984	3072	3077	3079	rBV4	1401	1355	0.07%	0.009%
69	11.035	3091	3093	3094	rBV2	1539	555	0.03%	0.004%
70	11.067	3101	3103	3106	rBV3	1887	1099	0.06%	0.007%
71	11.096	3110	3112	3115	rBV3	1557	1069	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015194.D
 Acq On : 27 Mar 2020 04:16
 Operator : SY/MD
 Sample : VV0326WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK94

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.273	3155	3167	3185	rBV	1186755	1792998	93.79%	11.518%
73	11.408	3207	3209	3213	rVB4	2215	1044	0.05%	0.007%
74	11.482	3230	3232	3235	rVB3	1785	765	0.04%	0.005%
75	11.592	3262	3266	3269	rBV6	2094	1597	0.08%	0.010%
76	11.646	3270	3283	3306	rVV	847355	1360698	71.18%	8.741%
77	11.897	3357	3361	3365	rBV6	1227	1178	0.06%	0.008%
78	11.974	3381	3385	3386	rBV4	1093	698	0.04%	0.004%
79	11.984	3386	3388	3390	rVB3	2504	1103	0.06%	0.007%
80	12.006	3390	3395	3399	rBV7	1747	2013	0.11%	0.013%
81	12.051	3405	3409	3411	rBV4	1977	1476	0.08%	0.009%
82	12.103	3424	3425	3427	rBV2	1044	452	0.02%	0.003%
83	12.157	3438	3442	3444	rBV4	1969	1509	0.08%	0.010%
84	12.309	3487	3489	3495	rBV7	1312	1016	0.05%	0.007%
85	12.508	3549	3551	3553	rBV3	1588	672	0.04%	0.004%
86	12.591	3575	3577	3578	rBV2	1198	549	0.03%	0.004%
87	12.604	3578	3581	3582	rBV3	1640	864	0.05%	0.006%
88	12.675	3596	3603	3606	rBV7	5874	7048	0.37%	0.045%
89	12.755	3624	3628	3633	rBV8	2658	2846	0.15%	0.018%
90	12.813	3642	3646	3648	rBV4	1989	1404	0.07%	0.009%
91	12.913	3673	3677	3679	rBV4	2195	1546	0.08%	0.010%
92	13.087	3729	3731	3740	rVB9	2594	3035	0.16%	0.019%
93	13.122	3740	3742	3744	rBV3	1184	749	0.04%	0.005%
94	13.132	3744	3745	3750	rVB4	1888	1440	0.08%	0.009%
95	13.154	3750	3752	3755	rBV3	1316	946	0.05%	0.006%
96	13.527	3862	3868	3870	rBV5	9728	9137	0.48%	0.059%
97	13.614	3893	3895	3897	rBV3	1826	960	0.05%	0.006%
98	13.971	4003	4006	4007	rBV3	1785	1065	0.06%	0.007%
99	14.083	4039	4041	4045	rBV5	2009	1578	0.08%	0.010%
100	14.235	4085	4088	4091	rBV5	2204	1526	0.08%	0.010%


Sum of corrected areas: 15566490

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015194.D
Acq On : 27 Mar 2020 04:16
Operator : SY/MD
Sample : VV0326WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK94

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

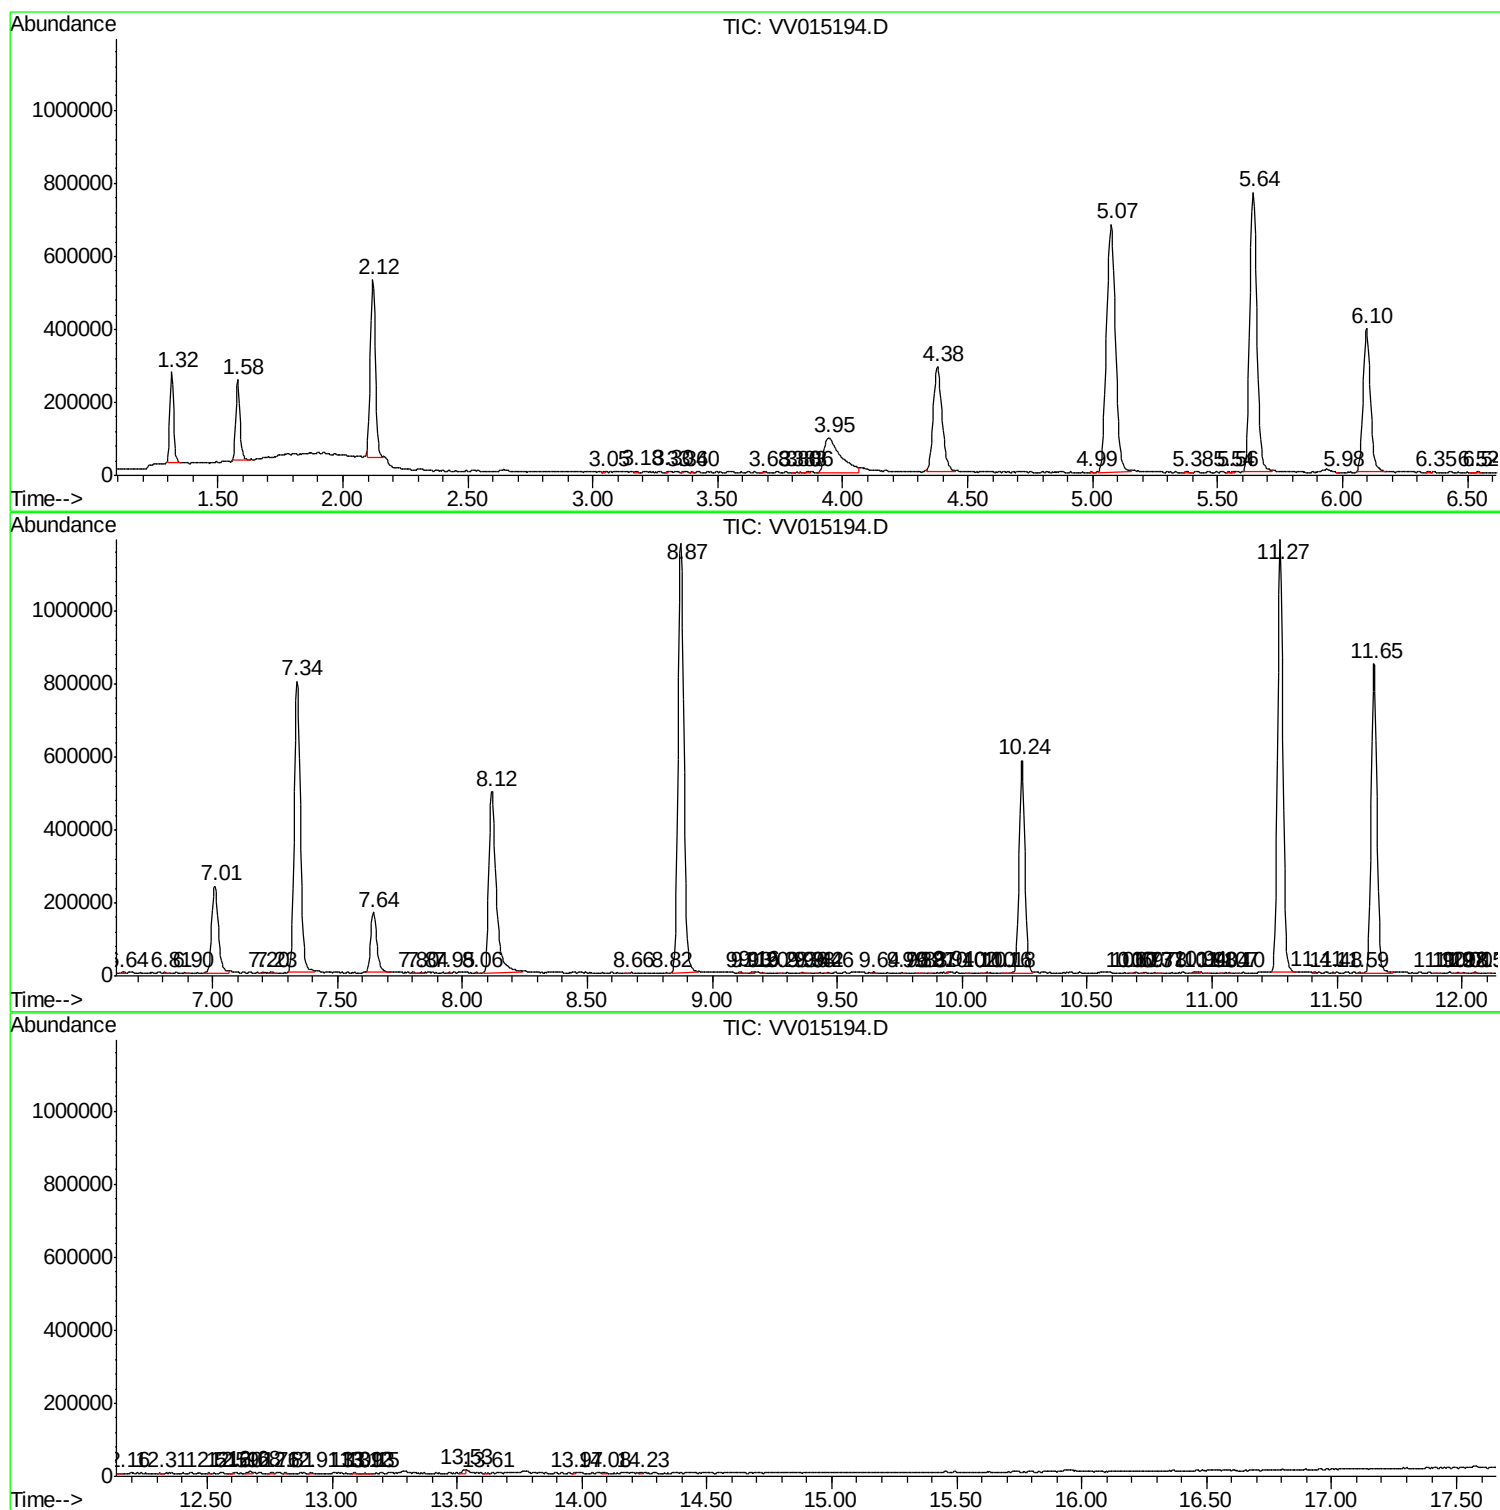

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015194.D
Acq On : 27 Mar 2020 04:16
Operator : SY/MD
Sample : VV0326WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK94

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015194.D
Acq On : 27 Mar 2020 04:16
Operator : SY/MD
Sample : VV0326WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK94

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc