

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015197.D
 Acq On : 27 Mar 2020 06:10
 Operator : SY/MD
 Sample : L1976-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	83	rVB2	314668	335598	12.28%	1.633%
2	1.579	147	152	163	rVB	225073	251444	9.20%	1.223%
3	2.122	314	321	331	rVB	440667	613989	22.47%	2.987%
4	3.277	676	680	687	rBV9	3068	3713	0.14%	0.018%
5	3.370	704	709	712	rBV8	2921	2308	0.08%	0.011%
6	3.454	734	735	741	rVB6	2348	1529	0.06%	0.007%
7	3.508	748	752	753	rBV4	1308	986	0.04%	0.005%
8	3.540	760	762	763	rBV2	1849	743	0.03%	0.004%
9	3.618	783	786	788	rBV3	2843	1495	0.05%	0.007%
10	3.701	810	812	816	rBV5	1368	949	0.03%	0.005%
11	3.939	870	886	916	rBV2	1065149	2732680	100.00%	13.294%
12	4.380	1009	1023	1045	rVB	312843	774794	28.35%	3.769%
13	4.759	1137	1141	1144	rBV6	2440	2239	0.08%	0.011%
14	4.904	1183	1186	1189	rBV5	2151	1622	0.06%	0.008%
15	4.939	1195	1197	1201	rBV4	1763	1269	0.05%	0.006%
16	4.987	1209	1212	1215	rBV5	2066	1414	0.05%	0.007%
17	5.074	1220	1239	1265	rBV2	749603	1890818	69.19%	9.198%
18	5.447	1350	1355	1361	rBV10	2663	4103	0.15%	0.020%
19	5.595	1399	1401	1402	rBV2	2018	954	0.03%	0.005%
20	5.643	1403	1416	1434	rVV	715913	1410206	51.61%	6.860%
21	5.939	1490	1508	1527	rBV	1235848	2380864	87.13%	11.582%
22	6.097	1545	1557	1585	rVB	446144	902033	33.01%	4.388%
23	6.386	1643	1647	1649	rBV5	1784	1336	0.05%	0.006%
24	6.598	1711	1713	1717	rVB5	1935	844	0.03%	0.004%
25	6.617	1717	1719	1721	rBV3	1781	848	0.03%	0.004%
26	6.637	1721	1725	1726	rBV4	1672	1194	0.04%	0.006%
27	6.765	1763	1765	1769	rVB4	2736	2065	0.08%	0.010%
28	6.785	1769	1771	1772	rBV2	1282	604	0.02%	0.003%
29	6.859	1792	1794	1796	rBV3	1926	952	0.03%	0.005%
30	7.010	1830	1841	1863	rBV	177315	316580	11.58%	1.540%
31	7.167	1886	1890	1893	rBV5	2458	1936	0.07%	0.009%
32	7.338	1932	1943	1964	rBV	869214	1498318	54.83%	7.289%
33	7.643	2028	2038	2057	rBV	131606	233668	8.55%	1.137%
34	7.830	2094	2096	2099	rBV4	1383	951	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015197.D
 Acq On : 27 Mar 2020 06:10
 Operator : SY/MD
 Sample : L1976-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	7.881	2108	2112	2115	rVB6	1845	1428	0.05%	0.007%
36	7.897	2115	2117	2120	rBV4	1952	1250	0.05%	0.006%
37	7.932	2126	2128	2131	rBV4	1630	1159	0.04%	0.006%
38	8.116	2173	2185	2221	rBV2	562074	1180857	43.21%	5.745%
39	8.331	2250	2252	2253	rBV2	1765	762	0.03%	0.004%
40	8.402	2273	2274	2277	rBV2	1730	757	0.03%	0.004%
41	8.447	2286	2288	2290	rBV3	1752	929	0.03%	0.005%
42	8.621	2339	2342	2346	rBV5	2151	1846	0.07%	0.009%
43	8.691	2363	2364	2366	rBV2	1352	624	0.02%	0.003%
44	8.727	2372	2375	2378	rBV4	1278	873	0.03%	0.004%
45	8.794	2393	2396	2398	rBV3	2326	1473	0.05%	0.007%
46	8.817	2401	2403	2405	rBV3	2053	900	0.03%	0.004%
47	8.875	2408	2421	2447	rBV	1120359	1810663	66.26%	8.808%
48	9.074	2481	2483	2485	rBV2	1265	701	0.03%	0.003%
49	9.228	2528	2531	2532	rBV3	1514	695	0.03%	0.003%
50	9.350	2566	2569	2571	rBV4	1633	845	0.03%	0.004%
51	9.457	2601	2602	2606	rVB3	2301	1053	0.04%	0.005%
52	9.479	2606	2609	2612	rBV3	2459	2009	0.07%	0.010%
53	9.527	2619	2624	2626	rBV6	1461	1237	0.05%	0.006%
54	9.543	2626	2629	2631	rBV4	1402	947	0.03%	0.005%
55	9.614	2649	2651	2657	rVB6	2006	2079	0.08%	0.010%
56	9.646	2657	2661	2664	rBV5	2448	2062	0.08%	0.010%
57	9.730	2686	2687	2689	rBV2	1200	577	0.02%	0.003%
58	9.788	2701	2705	2708	rBV4	2004	1482	0.05%	0.007%
59	9.891	2735	2737	2740	rVB4	1196	527	0.02%	0.003%
60	9.903	2740	2741	2743	rBV2	2094	886	0.03%	0.004%
61	10.074	2791	2794	2796	rBV4	1425	1027	0.04%	0.005%
62	10.103	2801	2803	2806	rBV3	974	592	0.02%	0.003%
63	10.238	2835	2845	2860	rVB	679732	1043652	38.19%	5.077%
64	10.325	2870	2872	2876	rBV4	1676	1070	0.04%	0.005%
65	10.447	2908	2910	2912	rBV3	1370	778	0.03%	0.004%
66	10.611	2956	2961	2965	rBV8	1896	1931	0.07%	0.009%
67	10.630	2965	2967	2969	rVV3	2265	1231	0.05%	0.006%
68	10.643	2969	2971	2974	rVB3	3715	1989	0.07%	0.010%
69	10.665	2974	2978	2979	rBV4	1916	1078	0.04%	0.005%
70	10.768	3007	3010	3013	rBV6	1023	675	0.02%	0.003%
71	10.910	3052	3054	3057	rBV4	1764	1156	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015197.D
 Acq On : 27 Mar 2020 06:10
 Operator : SY/MD
 Sample : L1976-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.122	3112	3120	3123	rBV8	2542	2770	0.10%	0.013%
73	11.193	3140	3142	3145	rBV4	2599	2057	0.08%	0.010%
74	11.273	3155	3167	3183	rBV	1034276	1587943	58.11%	7.725%
75	11.559	3244	3256	3270	rBV3	15102	30252	1.11%	0.147%
76	11.649	3270	3284	3299	rBV	916845	1445956	52.91%	7.034%
77	11.932	3368	3372	3375	rBV6	1678	1875	0.07%	0.009%
78	12.016	3397	3398	3402	rVB3	2255	1286	0.05%	0.006%
79	12.080	3416	3418	3419	rBV2	1867	608	0.02%	0.003%
80	12.164	3442	3444	3445	rBV2	1520	546	0.02%	0.003%
81	12.267	3473	3476	3477	rBV3	2014	1139	0.04%	0.006%
82	12.344	3497	3500	3502	rBV4	1865	1018	0.04%	0.005%
83	12.527	3550	3557	3558	rBV6	2366	2671	0.10%	0.013%
84	12.569	3568	3570	3573	rVB4	1694	683	0.02%	0.003%
85	12.598	3577	3579	3581	rBV3	2792	1595	0.06%	0.008%
86	12.665	3596	3600	3603	rBV5	2721	2631	0.10%	0.013%
87	12.839	3647	3654	3658	rBV9	2626	3142	0.11%	0.015%
88	12.913	3674	3677	3680	rBV4	2643	1551	0.06%	0.008%
89	12.932	3681	3683	3687	rVB5	1911	938	0.03%	0.005%
90	13.019	3706	3710	3712	rBV5	1177	987	0.04%	0.005%
91	13.144	3745	3749	3750	rBV3	1916	1496	0.05%	0.007%
92	13.189	3761	3763	3764	rBV2	2005	892	0.03%	0.004%
93	13.440	3838	3841	3843	rBV4	2825	1563	0.06%	0.008%
94	13.653	3904	3907	3910	rBV5	2780	2036	0.07%	0.010%
95	13.894	3979	3982	3986	rVB5	2244	1703	0.06%	0.008%
96	13.913	3986	3988	3990	rBV3	1378	669	0.02%	0.003%
97	14.022	4018	4022	4027	rBV6	2057	2434	0.09%	0.012%
98	14.074	4034	4038	4043	rBV7	2236	2632	0.10%	0.013%
99	14.550	4178	4186	4189	rBV10	2578	3164	0.12%	0.015%
100	14.669	4221	4223	4226	rBV4	1981	1098	0.04%	0.005%


Sum of corrected areas: 20556181

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015197.D
Acq On : 27 Mar 2020 06:10
Operator : SY/MD
Sample : L1976-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

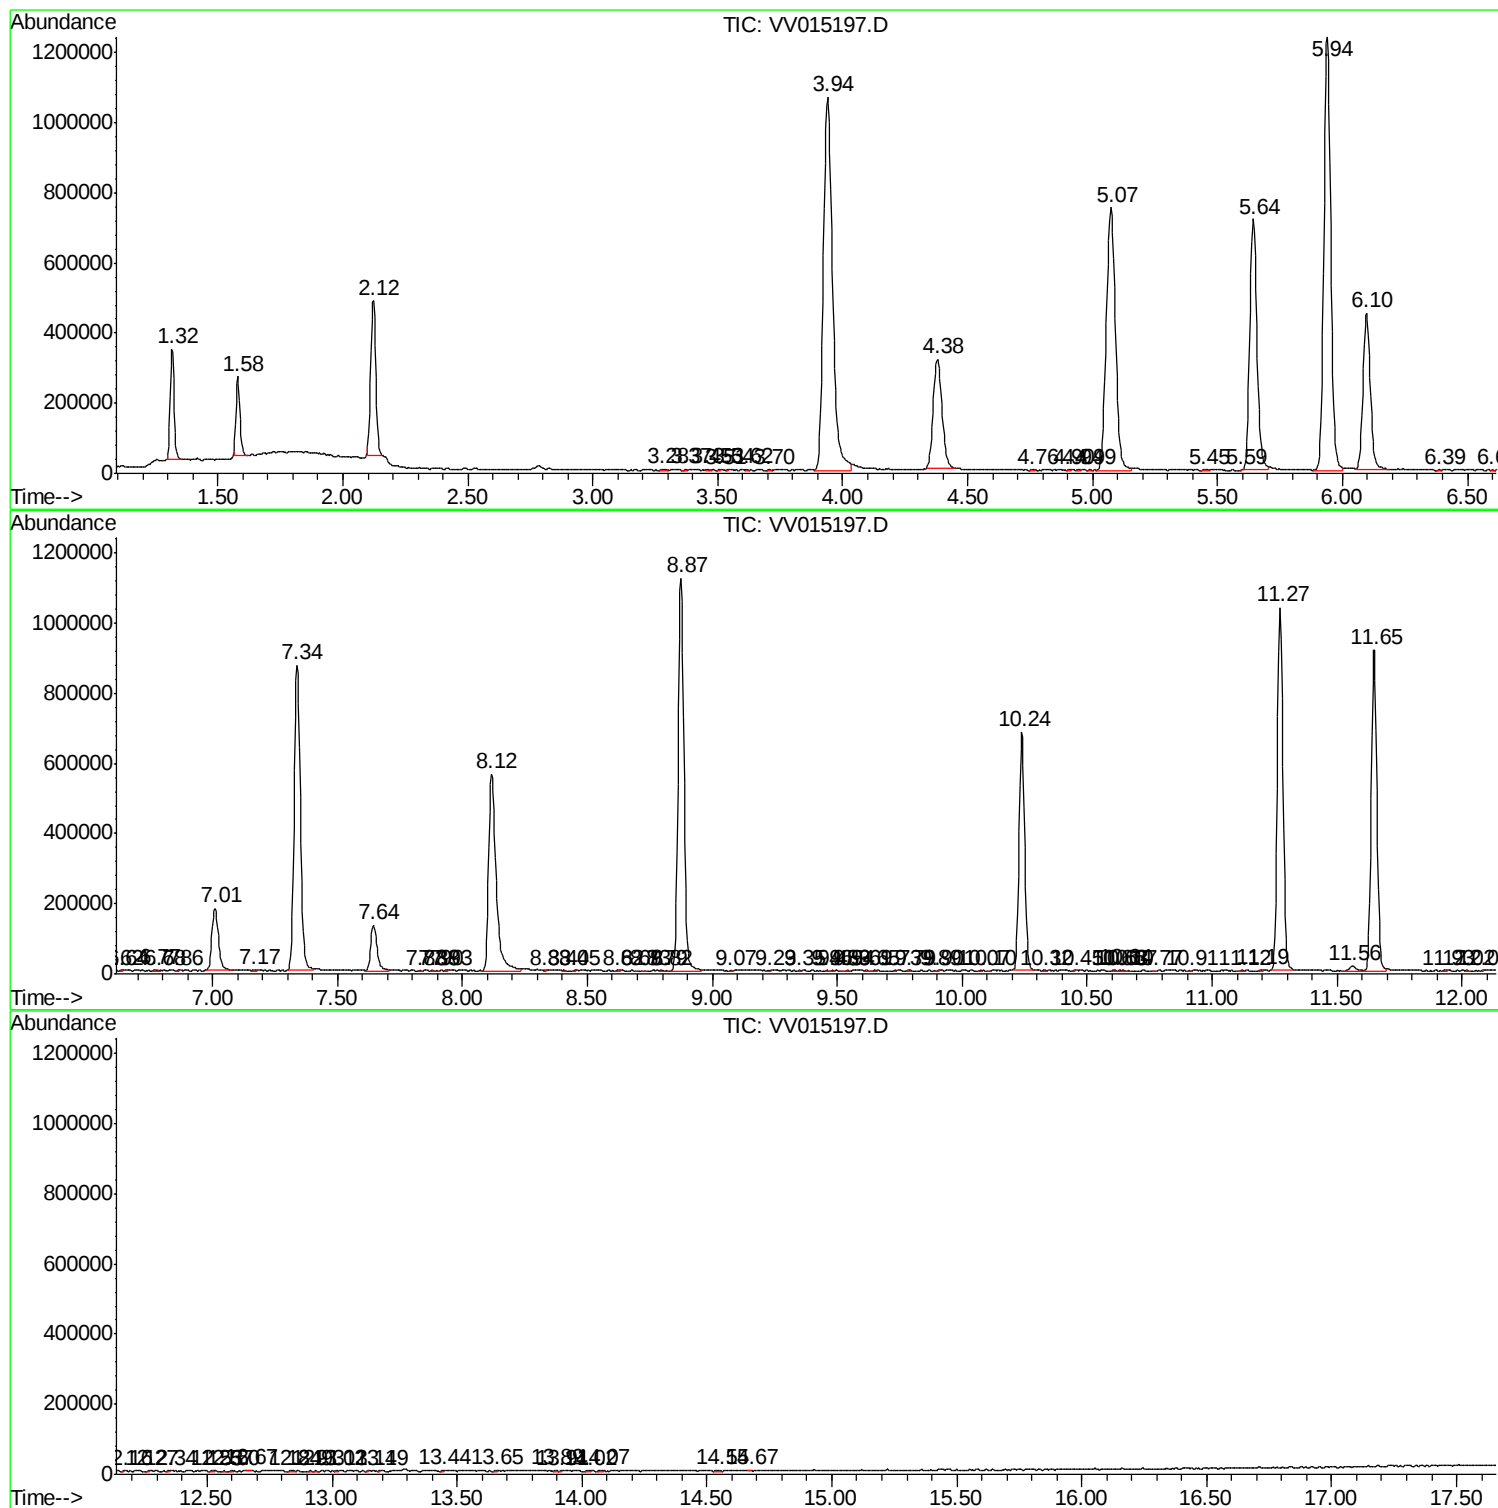

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015197.D
Acq On : 27 Mar 2020 06:10
Operator : SY/MD
Sample : L1976-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015197.D
Acq On : 27 Mar 2020 06:10
Operator : SY/MD
Sample : L1976-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
